


GE Healthcare
Life Sciences




Size Exclusion Chromatography

Principles and Methods

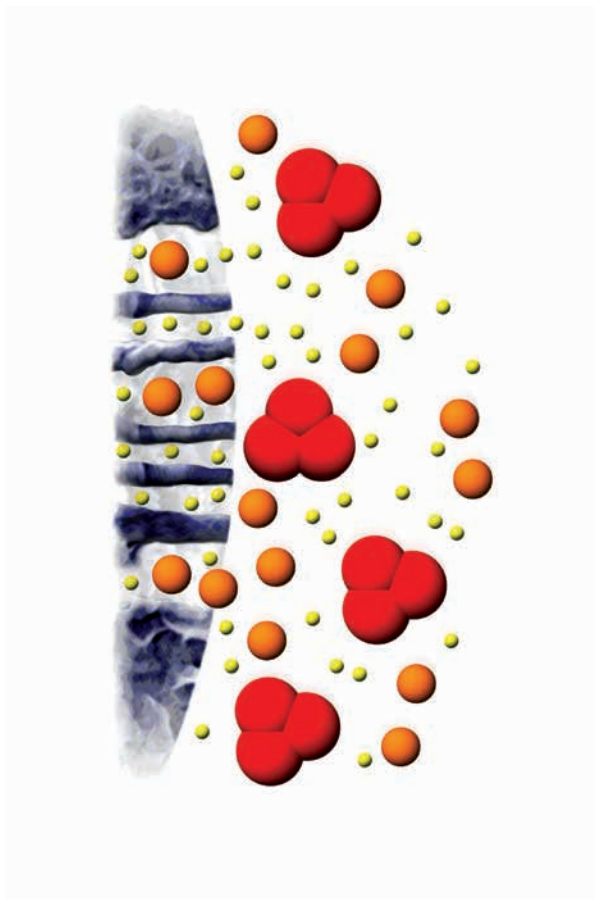

Handbooks from GE Healthcare Life Sciences

For more information refer to www.gelifesciences.com/handbooks




2-D Electrophoresis using Immobilized pH Gradients
Principles and Methods
80-6429-60




GST Gene Fusion System
Handbook
18-1157-58



Nucleic Acid Sample Preparation for Downstream Analyses
Principles and Methods
28-9624-00



Affinity Chromatography
Principles and Methods
18-1022-29




High-throughput Process Development with PreDictor Plates
Principles and Methods
28-9403-58



Protein Sample Preparation
Handbook
28-9887-41




ÄKTA Laboratory-scale Chromatography Systems
Instrument Management
Handbook
29-0108-31



Hydrophobic Interaction and Reversed Phase Chromatography
Principles and Methods
11-0012-69



Purifying Challenging Proteins
Principles and Methods
28-9095-31




Antibody Purification
Handbook
18-1037-46



Imaging
Principles and Methods
29-0203-01




Recombinant Protein Purification Handbook
Principles and Methods
18-1142-75




Biacore Assay
Handbook
29-0194-00



Ion Exchange Chromatography and Chromatofocusing
Principles and Methods
11-0004-21




Spectrophotometry
Handbook
29-0331-82



Biacore Sensor Surface
BR-1005-71



Isolation of Mononuclear Cells
Methodology and Applications
18-1152-69




Strategies for Protein Purification
Handbook
28-9833-31




Cell Separation Media
Methodology and Applications
18-1115-69




Microcarrier Cell Culture
Principles and Methods
18-1140-62



Western Blotting
Principles and Methods
28-9998-97



Size Exclusion Chromatography
Principles and Methods
18-1022-18



Multimodal Chromatography
Handbook
29-0548-08

Size exclusion chromatography

Principles and Methods

Contents

Introduction	7
Symbols	8
Common acronyms and abbreviations.....	9
Chromatography terminology.....	10
Chapter 1	
Size exclusion chromatography (SEC) in practice.....	15
Introduction.....	15
Purification by SEC	15
Group separation	16
High-resolution fractionation	17
Rapid purity check and screening.....	18
Resolution in SEC.....	18
Sample volume and column dimensions.....	18
Media selection.....	20
Sample and buffer preparation	24
Sample buffer composition	24
Sample concentration and viscosity	24
Sample volume.....	26
Buffer composition	26
Denaturing (chaotropic) agents and detergents.....	26
Column and media preparation	27
Setting column pressure limits.....	28
Sample application	30
Elution and flow rates.....	30
Controlling flow rates	32
Method development for high-resolution fractionation.....	32
Maintenance of SEC columns	33
Equipment selection.....	33
Scaling up.....	33
BioProcess media for large-scale production	34
Troubleshooting.....	35
Chapter 2	
Superdex: for high resolution, short run times, and high recovery	39
Superdex Increase	40
Superdex	42
Superdex prep grade.....	43
Separation options.....	45
Separation examples	46
Performing a separation	48
First-time use or after long-term storage.....	48
Cleaning.....	49
Removing severe contamination.....	49
Media characteristics.....	50
Chemical stability	50
Storage.....	50

Chapter 3

Superose: broad fractionation range for laboratory scale	51
Superose Increase	51
Superose.....	53
Superose prep grade	53
Separation options.....	54
Separation examples.....	55
Performing a separation	56
First-time use or after long-term storage.....	56
Cleaning.....	57
Media characteristics.....	57
Chemical stability	57
Storage.....	57

Chapter 4

Sephacryl: fast, high-recovery separations at laboratory and industrial scale.....	59
Separation options.....	62
Separation examples.....	63
Performing a separation	64
First-time use or after long-term storage.....	64
Cleaning.....	64
To remove severe contamination.....	65
Media characteristics.....	65
Chemical stability	65
Storage.....	66

Chapter 5

Sephadex: desalting, buffer exchange, and sample clean up	67
Separation options.....	68
Separation examples.....	72
Performing a separation	73
General considerations.....	73
Small-scale desalting of samples.....	73
Desalting larger sample volumes using HiTrap and HiPrep columns.....	73
Buffer preparation	74
Sample preparation	74
Buffer exchange	74
HiTrap Desalting columns.....	74
Manual purification with a syringe	75
Simple desalting with ÄKTAprime plus.....	76
Desalting on a gravity-feed PD-10 column	77
Buffer preparation	77
Optimization of desalting.....	77
Scale-up and processing larger sample volumes	78
Increasing sample loading capacity from 1.5 ml up to 7.5 ml.....	79
Increasing sample loading capacity from 15 ml up to 60 ml.....	79
For sample volumes greater than 60 ml.....	80
Media characteristics.....	80
Column packing	81
Cleaning.....	81
Chemical stability	81
Storage.....	81

Chapter 6	
Sephadex LH-20: size exclusion chromatography in organic solvents.....	83
Media characteristics.....	83
Separation examples	84
Packing a column	85
Performing a separation	86
Cleaning	86
Chemical stability.....	87
Storage	87
Transferring Sephadex LH-20 from aqueous solution to organic solvents	87
Chapter 7	
Size exclusion chromatography in theory.....	89
Defining the process.....	89
Selectivity curves and media selection	91
Resolution.....	92
Chapter 8	
Size exclusion chromatography in a purification strategy.....	95
The purification strategy according to CIPP.....	95
Purification of humanized IgG ₄ monoclonal antibody.....	97
Appendix 1	
Column packing and preparation.....	99
Columns for packing SEC media.....	99
Checking column efficiency.....	100
Column packing for high-resolution fractionation using Superdex prep grade and Sephacryl High Resolution	101
Column packing for group separations using Sephadex	103
Controlling flow rates.....	105
Appendix 2	
Sephadex and Darcy's law	106
Appendix 3	
Sample preparation	107
Sample clarification.....	107
Centrifugation.....	107
Filtration.....	107
Desalting	108
Denaturation.....	108
Precipitation and resolubilization.....	108
Ammonium sulfate precipitation	109
Removal of lipoproteins.....	111
Appendix 4	
Selection of purification equipment.....	112
System recommendations for high-resolution SEC columns.....	112

Appendix 5	
Converting from linear flow (cm/h) to volumetric flow rates (ml/min) and vice versa	114
From linear flow (cm/h) to volumetric flow rate (ml/min)	114
From volumetric flow rate (ml/min) to linear flow (cm/h)	114
From ml/min to using a syringe	115
Appendix 6	
Conversion data	116
Proteins	116
Nucleic Acids	116
Column pressures	116
Appendix 7	
Amino acids table	118
Appendix 8	
Analysis and characterization	120
Protein detection and quantitation	120
Purity check and protein characterization	120
Purity	120
Characterization	121
Appendix 9	
Storage of biological samples	122
General recommendations	122
Common storage conditions for purified proteins	122
Appendix 10	
Molecular weight estimation and molecular weight distribution analysis	123
Performing a molecular weight determination	125
Related literature	128
Ordering information	129
High-resolution SEC	129
Desalting and group separations	130
Empty columns	131
Accessories and spare parts	132

Introduction

Biomolecules are purified using chromatography techniques that separate them according to differences in their specific properties, as shown in Figure I.1.

Property	Technique
Size	Size exclusion chromatography (SEC), also called gel filtration (GF)
Hydrophobicity	Hydrophobic interaction chromatography (HIC) Reversed phase chromatography (RPC)
Charge	Ion exchange chromatography (IEX)
Biorecognition (ligand specificity)	Affinity chromatography (AC)
Isoelectric point (pI)	Chromatofocusing (CF)

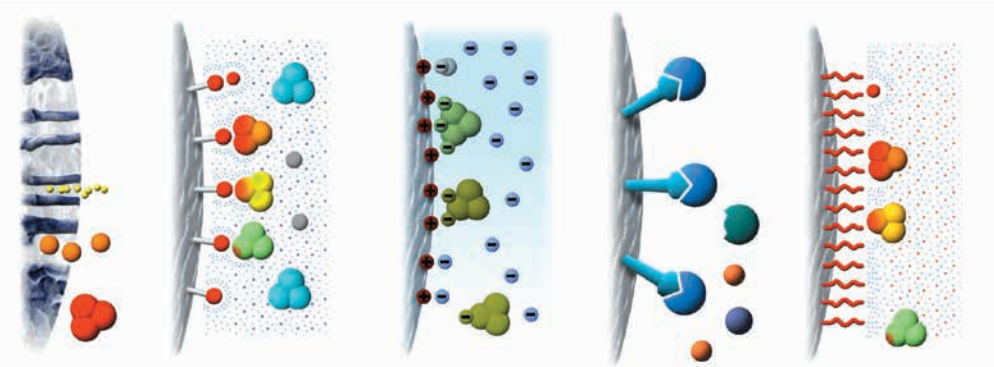


Fig I.1. Schematic drawing of separation principles in chromatography purification. From left to right: SEC, HIC, IEX, AC, and RPC.

Since the introduction of Sephadex™ chromatography medium (also known as resin) more than 50 years ago, SEC has played a key role in the purification of proteins and enzymes, polysaccharides, nucleic acids, and other biological macromolecules. SEC is the simplest and mildest of all the chromatography techniques and separates molecules on the basis of differences in size. The technique can be applied in two distinct ways:

1. **Group separations:** the components of a sample are separated into two major groups according to size range. A group separation can be used to remove high- or low-molecular weight contaminants (such as phenol red from culture fluids) or for desalting and buffer exchange (Fig I.2).

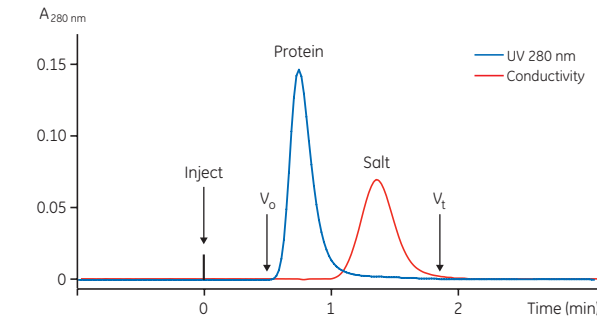


Fig I.2. Typical group separation.

2. **High-resolution fractionation of biomolecules:** the components of a sample are separated according to differences in their molecular size. High-resolution fractionation can be used to isolate one or more components, to separate monomers from aggregates, or to perform a molecular weight distribution analysis. High-resolution SEC is most suitable for samples that originally contain few components or for samples that have been partially purified by other chromatography techniques; this ensures that most of the unwanted proteins of similar size are eliminated (Fig I.3).

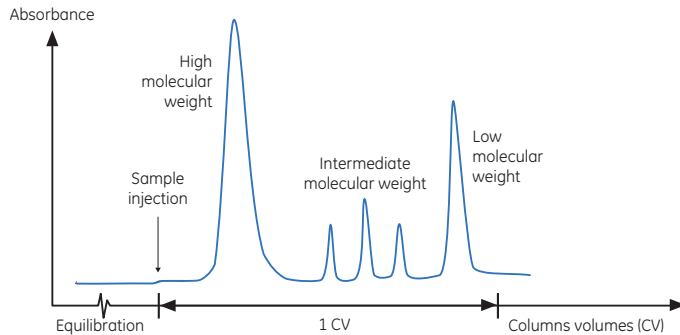


Fig I.3. Typical high-resolution SEC separation.

SEC can also facilitate the refolding of denatured proteins by careful control of changing buffer conditions.

This handbook describes the use of SEC for the purification and separation of biomolecules, with a focus on practical information for obtaining the best results. The media available, selection criteria and examples with detailed instructions for the most common applications are included, as well as the theoretical principles behind the technique. The first step towards a successful separation is to select the correct medium and this handbook focuses on the most up-to-date SEC media and prepacked columns.

Symbols



This symbol indicates general advice on how to improve procedures or recommends measures to take in specific situations



This symbol indicates where special care should be taken



Highlights chemicals, buffers, and equipment



Outline of experimental protocol.

Common acronyms and abbreviations

^3H	tritium
^{32}P	phosphorous 32
A_{280}	UV absorbance at specified wavelength (in this example, 280 nm)
AC	affinity chromatography
ALEX	anion exchange chromatography
A_s	peak symmetry, expressed as asymmetry factor
ATP	adenosine triphosphate
AU	absorbance units
BSA	bovine serum albumin
CF	chromatofocusing
CIEX	cation exchange chromatography
CIP	cleaning-in-place
CIPP	capture, intermediate purification, polishing
CV	column volume(s)
DDM	n-dodecyl- β -maltoside
DM	n-decyl- β -maltoside and
DNA	deoxyribonucleic acid
DoE	design of experiments
DTE	dithioerythritol
DTT	dithiothreitol
dTTP	2'-deoxythymidine triphosphate
EDTA	Ethylenediaminetetra acetic acid
ELISA	Enzyme-linked immunosorbent assay
GF	gel filtration (also referred to as SEC, size exclusion chromatography)
HCl	hydrochloric acid
HIC	hydrophobic interaction chromatography
HIV	human immunodeficiency virus
HMW	high molecular weight
HPLC	high-performance liquid chromatography
i.d.	inner diameter
ID_{50}	inhibitory dose causing 50% inhibition
IEF	isoelectric focusing
IEX	ion exchange chromatography
IGF-1	insulin-like growth factor 1
IgG	immunoglobulin G
IgM	immunoglobulin M
IMAC	immobilized metal affinity chromatography
IU	inhibitor activity units
K_{av}	partition coefficient
K_d	distribution coefficient
K_o	specific permeability
LMW	low molecular weight
mAU	milli absorbance units
MPa	megaPascal
M_p	peak molecular weight
M_r	relative molecular mass
MS	mass spectrometry
NaCl	sodium chloride
NHS	n-hydroxysuccinimide
Ni	nickel

N/m, Nm ⁻¹	column efficiency expressed as number of theoretical plates per meter
NM	n-nonyl-β-maltoside
PAGE	polyacrylamide gel electrophoresis
PBS	phosphate-buffered saline
pI	isoelectric point
psi	pounds per square inch
PVDF	polyvinylidene fluoride
RI	refractive index
RNA	ribonucleic acid
RPC	reversed phase chromatography
R _s	resolution, the degree of separation between peaks
SDS	sodium dodecyl sulfate
SEC	size exclusion chromatography (also referred to as GF, gel filtration)
ssDNA, ssRNA	single-stranded DNA, RNA
SR	solvent resistant
TCM	traditional Chinese medicine
UDM	n-undecyl-β-maltoside
UV	ultraviolet
V _e	peak elution (retention) volume
V ₀	void volume
V _i	volume of buffer inside the matrix
V _s	volume of stationary phase
V _{sep}	separation volume
V _t	total volume of the packed bed
v/v	volume/volume
W1/2	peak width at half peak height
w/v	weight/volume

Chromatography terminology

Adapter	Often used for the movable end pieces of columns; contains filter, flow distributor, and possibility to connect tubing.
Adsorption	Binding. The process of interaction between the solute (for example, a protein) and the stationary phase.
Affinity chromatography	A group of methods based on various types of specific affinities between target molecule(s), for example, a protein and a specific ligand coupled to a chromatography medium.
Asymmetry (asymmetry factor)	Factor describing the shape of a chromatographic peak.
Backpressure	The pressure drop across a column and/or a chromatography system.
Band broadening	The widening of a zone of solute (for example, a protein) when passing through a column or a chromatography system. Gives rise to dilution of the solute and reduces resolution. Also often called peak broadening or zone broadening.
Binding	Adsorption. The process of interaction between a solute (for example, a protein) and the stationary phase.
Binding buffer	Buffer/solution/eluent used for equilibration of the column before sample loading.

Binding capacity	The maximum amount of material that can be bound per ml of chromatography medium. See also Dynamic binding capacity.
Capacity factor	The degree of retention of a solute (for example, a protein) relative to an unretained peak.
Chromatofocusing	Method that separates proteins on the basis of pI.
Chromatogram	A graphical presentation of detector response(s) indicating the concentration of the solutes coming out of the column during the purification (volume or time).
Chromatography	From Greek chroma, color, and graphein, to write.
Chromatography medium/media	The stationary phase, also called resin. The chromatography medium is composed of a porous matrix that is usually functionalized by coupling of ligands to it. The matrix is in the form of particles (beads) or, rarely, a single polymer block (monolith).
CIP (cleaning-in-place)	Common term for cleaning chromatography columns and/or systems with the purpose of removing unwanted/nonspecifically bound material.
Column	Usually column hardware packed with chromatography medium.
Column equilibration	Passage of buffer/solution through the chromatography column to establish conditions suitable for binding of selected sample components. For example, to establish correct pH and ionic strength, and ensure that proper counter ions or counter ligands are present.
Column hardware	The column tube and adapters. All pieces of the column except the chromatography medium/the packed bed.
Column hardware pressure	The pressure inside the column. Column hardware pressure that is too high can break the column.
Column packing	Controlled filling of the column hardware with chromatography medium to obtain a packed bed.
Column volume	The geometrical volume of the column interior/the chromatography bed.
Counter ion	Ion of opposite charge that interacts with an ion exchange chromatography medium after the column equilibration. The counter ion is displaced by a protein that binds to the ion exchanger. If a high concentration of the counter ion is applied, it will compete with the bound protein and elute it from the chromatography column.
Counter ligand	Substances that interact with ligands of a chromatography medium and can be displaced by a solute (for example, protein) binding to the ligand.
Dead volume	The volume outside the packed chromatography bed. Can be column dead volume or chromatography system dead volume. The dead volume contributes to band broadening.
Degassing	Removal of dissolved air from buffers/solutions.
Desorption	Elution. Release or removal of bound substances from the chromatography medium.

Design of experiments (DoE)	DoE allows use of a minimum number of experiments, in which several experimental parameters can be varied simultaneously. Based on the obtained data, a mathematical model of the studied process (e.g., a protein purification protocol or a chromatography step) is created. The model can be used to understand the influence of the experimental parameters on the outcome and to find an optimum for the process.
Dynamic binding capacity	The binding capacity determined by applying the target using flow through a column, as opposed to equilibrium binding capacity determined by batch experiment.
Efficiency	Measured as number of theoretical plates. High efficiency means that sharp peaks will be obtained.
Effluent	The mobile phase leaving the column (= eluate).
Eluate	The mobile phase leaving the column (= effluent).
Eluent	The buffer/solution used during chromatography (= mobile phase).
Elution buffer	Buffer/solution used for elution (desorption) of bound solutes (for example, proteins) from a column.
Elution volume	The volume of buffer/solution (eluent) required to elute the solute for example, a protein (= retention volume).
Elution time	The time required for elution of a solute (protein) (= retention time).
Flow rate	Volumetric flow (ml/min) or linear flow rate (cm/h). Measurement of flow through a column and/or chromatography system.
Flowthrough	Material passing the column during sample loading (without being bound).
Frit	Type of deep filter often used at top and bottom of columns.
Gel filtration (GF)	Size-exclusion chromatography. Separates solutes (for example, proteins) according to size.
Gradient elution	Continuous increased or decreased concentration of a substance (in the eluent) that causes elution of bound solutes (for example, proteins).
Hydrophobic interaction chromatography (HIC)	Method based on the hydrophobic interaction between solutes (for example, proteins) and the chromatography medium in the presence of high salt concentration.
Hydroxyapatite chromatography	Mixed-mode ion exchange chromatography method.
Immobilized metal ion affinity chromatography (IMAC)	Method based on the affinity of proteins with His, Cys, or Trp amino residues on their surface and metal ions on the chromatography medium.
Ion exchange chromatography (IEX)	Method based on electrostatic interactions between solutes (for example, proteins) and chromatography medium.
Isocratic elution	Elution of the solutes without changing the composition of the buffer/solution (eluent).
Ligand	The specific molecular group that is coupled to the matrix to give some decided function to the chromatography medium.
Ligand density	Related to ligand concentration. The distribution of ligands on the surfaces (also surfaces inside pores) of the chromatography matrix.
Linear velocity	The flow rate normalized by the column cross section (cm/h).

Mass transfer	Movement of a solute (for example, a protein) in and out of the stationary phase. Important factor for column efficiency.
Matrix	The matrix is the nonfunctional base for the chromatography medium. The matrix has a porous structure that provides a large surface that can be modified with ligands that introduce possibilities for protein binding.
Mobile phase	The fluid (buffer/solution) carrying the solutes during chromatography (= eluent).
Peak broadening	Same as band broadening.
Peak capacity	The number of peaks that can be separated using a chromatography column.
Peak tailing	Broadening at the end of a peak due to additional delay of a fraction of the solute. Results in increased asymmetry factor.
Pore	Cavity in a chromatography matrix.
Pore volume	The total volume of the pores in a chromatography medium.
Pressure over the packed bed	The pressure drop across the packed bed upon passage of solution through the column. Caused by flow resistance in the packed bed.
Recovery	The relative amount of target protein that is retrieved after purification compared with amount loaded on the column.
Resin	The term is sometimes used instead of the more generic term, chromatography medium.
Resolution	Measurement of the ability of a packed column to separate two solutes (peaks).
Retention volume	Same as elution volume.
Retention time	Same as elution time.
Reversed phase chromatography (RPC)	Method based on hydrophobic interactions between solutes (sample components) and ligands coupled to the chromatography medium. Organic modifiers (for example, acetonitrile) in the eluent are used for elution.
Sample	The material loaded on the chromatography column/medium, or to be analyzed.
Sample application	Applying/loading sample on the column.
Sample loading	Loading/applying sample on the column.
Sample volume	Usually the volume of the sample loaded on the chromatography column/medium.
Selectivity	Measure of the relative retention of two solutes in a column. Related to the distance between two peaks.
Solute	The dissolved substance (for example, a protein) in, for example, the mobile phase.
Stationary phase	Often called resin, chromatography beads, chromatography material, chromatography medium or media.
Step gradient elution	Stepwise increase in concentration of the substance that affects elution of bound solutes.
Void volume	The elution volume of solutes that do not enter the pores or interact with the chromatography medium, thus passing between the beads in the packed bed.
Wash	Wash step. Removal of unbound or weakly bound material from a column after the sample loading.

Wash buffer	Buffer/solution used for washing the column after sample loading.
Wash volume	Volume of buffer/solution used for the wash step.
Yield	Amount of target protein (or other solute) obtained after a purification step, or after the entire purification (multiple steps).
Zone broadening	Same as peak broadening.

Chapter 1

Size exclusion chromatography in practice

Introduction

SEC separates molecules according to differences in size as they pass through a SEC medium packed in a column. Unlike IEX or AC, molecules do not bind to the chromatography medium so buffer composition does not directly affect resolution (the degree of separation between peaks). Consequently, a significant advantage of SEC is that conditions can be varied to suit the type of sample or the requirements for further purification, analysis, or storage without altering the separation.

SEC is well-suited to biomolecules that are sensitive to changes in pH, concentration of metal ions, or cofactors and harsh environmental conditions. Separations can be performed in the presence of essential ions, cofactors, detergents, urea, or guanidine hydrochloride at high or low ionic strength; at 37°C or in the cold room according to the requirements of the experiment. Purified proteins can be collected in any chosen buffer.

This chapter provides general guidelines applicable to any SEC separation. A key step towards successful separation is selecting the correct medium; this handbook includes guides to the most up-to-date media and prepacked columns. Application examples and product-specific information are found in Chapters 2 to 6.

Purification by SEC

To perform a separation, the medium is packed into a column to form a packed bed. SEC media consist of a porous matrix of spherical particles with chemical and physical stability and inertness (lack of reactivity and adsorptive properties). The packed bed is equilibrated with buffer, which fills the pores of the matrix and the space between the particles. The liquid inside the pores, or stationary phase, is in equilibrium with the liquid outside the particles, or mobile phase. Samples are eluted isocratically so there is no need to use different buffers during the separation. However, a wash step using the running buffer is usually included at the end of a separation to remove molecules that might have been retained on the column and to prepare the column for a new run.

SEC can be used directly after IEX, CF, HIC, or AC since the buffer composition will not generally affect the final separation. For further details on using SEC in a purification strategy, refer to Chapter 8.

Figure 1.1 illustrates the separation process of SEC and the theory for this process is described in Chapter 7.

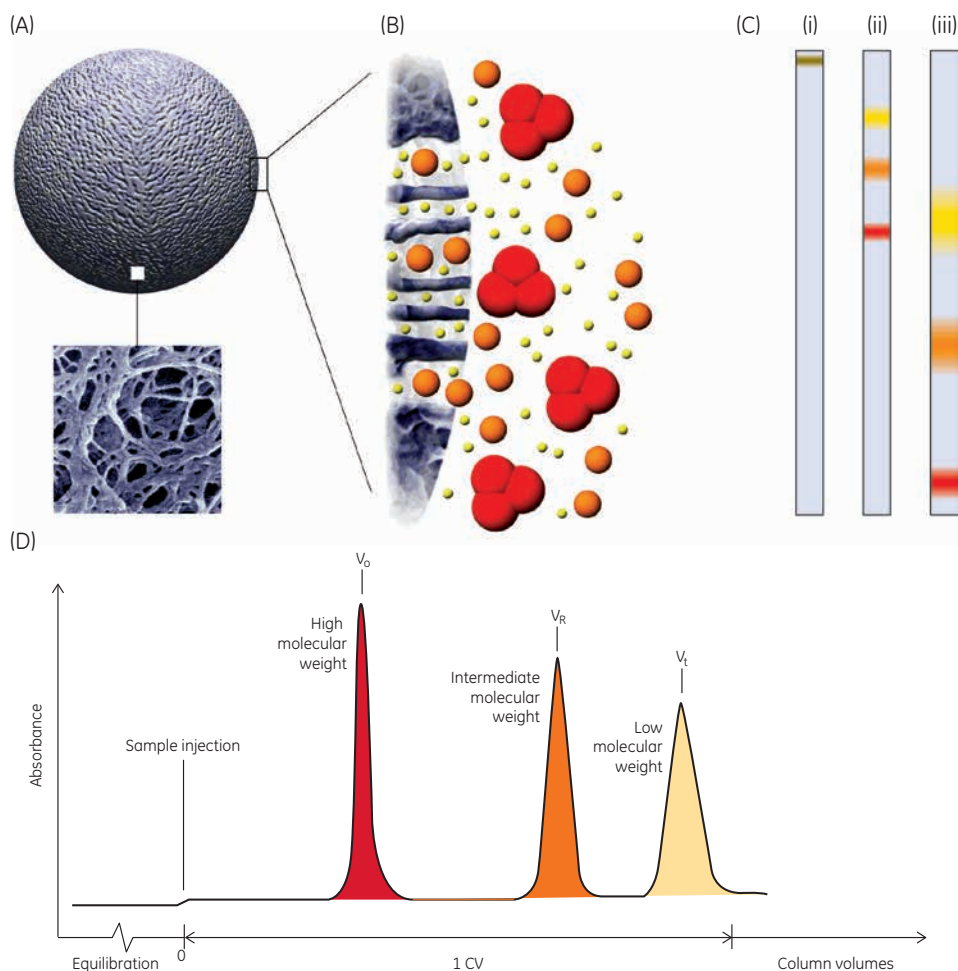


Fig 1.1. Process of SEC. (A) Schematic picture of a bead with an electron microscopical enlargement. (B) Schematic drawing of sample molecules diffusing into bead pores. (C) Graphical description of separation: (i) sample is applied on the column; (ii) the smallest molecule (yellow) is more delayed than the largest molecule (red); (iii) the largest molecule is eluted first from the column. Band broadening causes significant dilution of the protein zones during chromatography. (D) Schematic chromatogram.

Group separation

SEC is used in group separation mode to remove small molecules from a group of larger molecules and as a fast, simple solution for buffer exchange. Small molecules such as excess salt or free labels are easily separated from larger molecules. Samples can be prepared for storage or for other chromatography techniques and assays. SEC in group separation mode is often used in protein purification schemes for desalting and buffer exchange. Sephadex G-10, G-25, and G-50 are used for group separations. Large sample volumes, up to 30% of the total column volume (packed bed), can be applied at high flow rates using broad, short columns. Figure 1.2 shows the chromatogram (elution profile) of a typical group separation. Large molecules are eluted in or just after the void volume, V_0 , as they pass through the column at the same speed as the flow of buffer. For a well-packed column, V_0 is equivalent to approximately 30% of the total column volume. Small molecules such as salts that have full access to the pores move down the column, but do not separate from each other. These molecules usually elute just before one total column volume, V_L , of buffer has passed through the column. In this case the proteins are detected by monitoring their UV absorbance, usually at 280 nm, and the salts are detected by monitoring the conductivity of the buffer.

Column: HiTrap™ Desalting 5 ml
Sample: (Histidine)₆ protein eluted from HiTrap Chelating HP with
20 mM sodium phosphate, 500 mM sodium chloride
500 mM imidazole, pH 7.4
Buffer: 20 mM sodium phosphate, 150 mM sodium chloride, pH 7.0

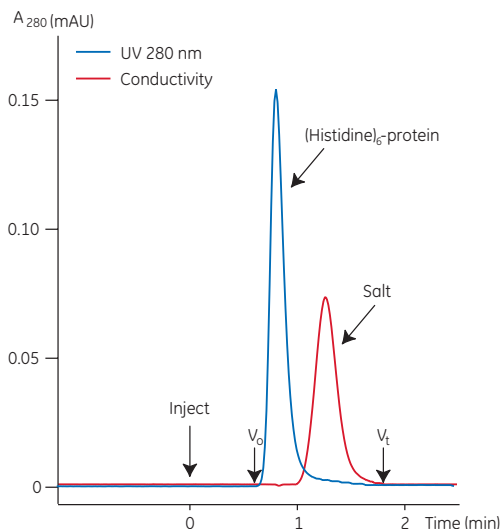


Fig 1.2. Typical chromatogram of a group separation. UV (protein) and conductivity (salt) detection enable pooling of the desalted fractions and facilitate optimization of the separation V₀ = void volume; V_t = total column volume.

Refer to Chapter 5 for detailed information on how Sephadex is used in group separation of high- and low-molecular weight substances in applications like desalting, buffer exchange, and sample clean up.

Refer to Chapter 7 for detailed information on the theory of SEC.

High-resolution fractionation

SEC is used in fractionation mode to separate multiple components in a sample on the basis of differences in their size. The goal can be to isolate one or more of the components, or to analyze the molecular-weight distribution in the sample. Optimal results for high-resolution fractionation will be achieved with samples that originally contain few components or with samples that have been partially purified by other chromatography techniques to eliminate most of the unwanted proteins of similar size.

High-resolution fractionation by SEC is well-suited for the final polishing step in a purification scheme. Monomers are easily separated from aggregates. Samples can be transferred to a suitable buffer for assay or storage.

Prepacked SEC columns are highly recommended for optimal performance during high-resolution fractionation and are available for three different purposes:

- Preparative purification for sample volumes in the milliliter range.
- Small-scale preparative purification for sample volumes up to 500 µl.
- Analytical runs for sample volumes up to 500 µl.

HiLoad™ columns prepacked with Superdex™ prep grade media, or HiPrep™ columns prepacked with Sephacryl™ media, are used for preparative purification, which is characterized by collection of the sample. The sample volume is in the milliliter range and the collected fractions are usually in milligram amounts.

Small-scale preparative purification and analytical runs are performed using Superdex or Superose™ media prepacked in Tricorn™ or Precision Columns (PC columns). Compared with preparative purification, the sample size and collected amounts are smaller (microliter and microgram to milligram scale) in small-scale preparative purification. Depending on sample volume, either Tricorn 10/300 GL columns should be used (25 µl to 500 µl) or 3.2/300 columns (4 µl to 50 µl). While samples are collected in preparative purification, no collection of sample in analytical purification is necessary—in this case it is the data from the run that is in focus.

Rapid purity check and screening

Short columns with small bed volumes such as Superdex 75 5/150 GL, Superdex 200 Increase 5/150 GL, and Superose 6 Increase 5/150 GL are suitable for rapid purity check or size analysis of proteins and other biomolecules. Short cycle times, together with small sample volume and low buffer consumption make this column a good choice in screening experiments to check protein homogeneity. However, when using the same media, shorter columns give lower resolution than longer columns.

Resolution in SEC

The success of SEC depends primarily on choosing conditions that give sufficient selectivity and counteract peak broadening effects during the separation. After selection of SEC medium, sample volume and column dimensions are the two most critical parameters that will affect the resolution of the separation. Chromatography system-related factors can also affect resolution.



The final resolution is influenced by many factors (Table 1.1). The molecular-weight range over which an SEC medium can separate molecules is referred to as the selectivity of the medium (see fractionation range guide for SEC media in *Media selection* in this chapter). Resolution is a function of the selectivity of the medium and the efficiency of that medium to produce narrow peaks (minimal peak broadening), as illustrated in Chapter 7.

Table 1.1. Factors that influence resolution

Medium-related factors	Particle size Particle uniformity Match between pore size and analyte size
Column-related factors	Bed height Column packing quality
Chromatography system-related factors	Tubing dimensions (diameter and length) Volumes in system components
Experimental-related factors	Flow rate Sample volume Viscosity

Sample volume and column dimensions

The sample volume can be expressed as a percentage of the total column volume (packed bed). Smaller sample volumes help to avoid overlap if closely spaced peaks are eluted. Figure 1.3 illustrates how sample volume can influence a high-resolution fractionation.

-  For group separations, use sample volumes up to 30% of the total column volume.
-  For high-resolution fractionation, a sample volume from 0.5% to 4% of the total column volume is recommended, depending on the type of medium used. For most applications the sample volume should not exceed 2% to achieve maximum resolution. Depending on the nature of the specific sample, it might be possible to load larger sample volumes, particularly if the peaks of interest are well resolved. This can only be determined by experimentation.

Column: Superdex 200 Increase 5/150 GL
Sample: 1. Thyroglobulin (M_r 669 000), 3 mg/ml
 2. Aldolase (M_r 158 000), 3 mg/ml
 3. Conalbumin (M_r 75 000), 3 mg/ml
 4. Carbonic anhydrase (M_r 29 000), 3 mg/ml
 5. Ribonuclease A (M_r 13 700), 3 mg/ml
Sample volume: 50 μ l and 4 μ l
Buffer: 10 mM phosphate buffer, 140 mM sodium chloride, pH 7.4
Flow rate: 0.45 ml/min, room temperature
System: ÄKTAmicro

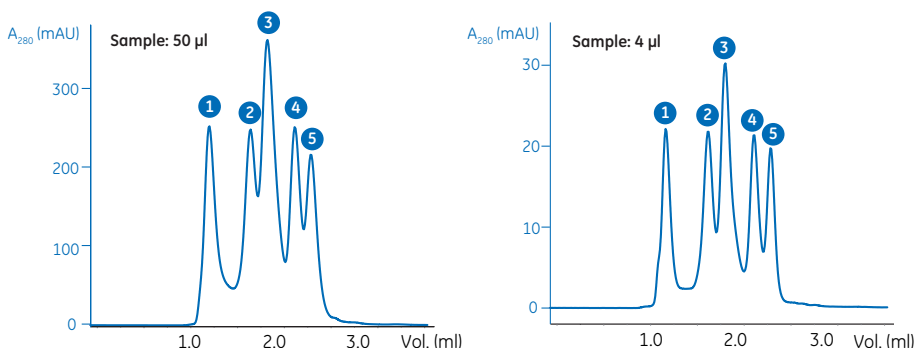


Fig 1.3. Comparison of protein separation on Superdex 200 Increase 5/150 GL using different sample volumes.



The ratio of sample volume to column volume influences resolution, as shown in Figure 1.4, where higher ratios give lower resolution. Column volumes are normally selected according to the sample volumes to be processed. Larger sample volumes can require significantly larger column volumes; it might be beneficial to repeat the separation several times on a smaller column and pool the fractions of interest or concentrate the sample (see Appendix 3).



For analytical separations and separations of complex samples, start with a sample volume of 0.5% of the total column volume. Sample volumes of less than 0.5% do not normally improve resolution.



Concentrating samples can increase the capacity of a SEC separation. Avoid concentrations above 70 mg/ml protein as viscosity effects can interfere with the separation.



Sample dilution is inevitable since diffusion occurs as sample passes through the column. To minimize sample dilution, use a sample volume that gives the resolution required between the peaks of interest.

Column: HiLoad 16/600 Superdex 200 prep grade
Sample: Solution of transferrin (M_r 81 000) and immunoglobulin G (IgG, M_r 160 000) by equal weight
Sample concentration: 8 mg/ml
Buffer: 50 mM sodium phosphate, 100 mM sodium chloride, pH 7.2
Flow rate: 1 ml/min (30 cm/h)

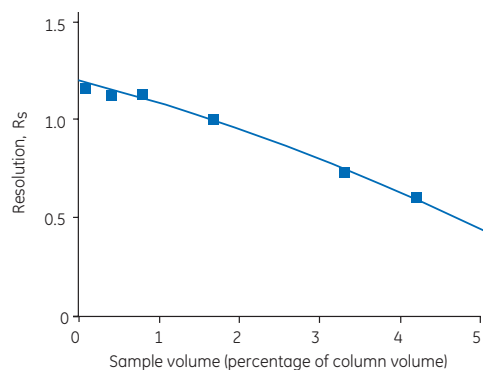


Fig 1.4. Influence of ratio of sample volume to column volume on the resolution of transferrin and IgG on prepacked HiLoad 16/60 Superdex 200 prep grade. Resolution is defined in Chapter 7.

The height of the packed bed affects both resolution and the time taken for elution. The resolution in SEC increases with the square root of bed height. Doubling the bed height gives an increase in resolution equivalent to $\sqrt{2} = 1.4$ (40%). For high resolution and fractionation, long columns will give the best results. Sufficient bed height together with a low flow rate allows time for 'intermediate' molecules to diffuse in and out of the matrix and give sufficient resolution.



If a very long column is necessary, the effective bed height can be increased by using columns, containing the same media, coupled in series.

Refer to Chapter 7 for detailed information on the theory of SEC.

Media selection

Today's SEC media cover a molecular weight range from 100 to 80 000 000, separating biomolecules from peptides to very large proteins and protein complexes.

The selectivity of a SEC medium depends solely on its pore size distribution and is described by a selectivity curve. SEC media are supplied with information about selectivity, as shown for Superdex in Figure 1.5. The curve is a plot of the partition coefficient K_{av} against the log of the molecular weight for a set of standard proteins (for calculation of K_{av} (see Chapter 7).

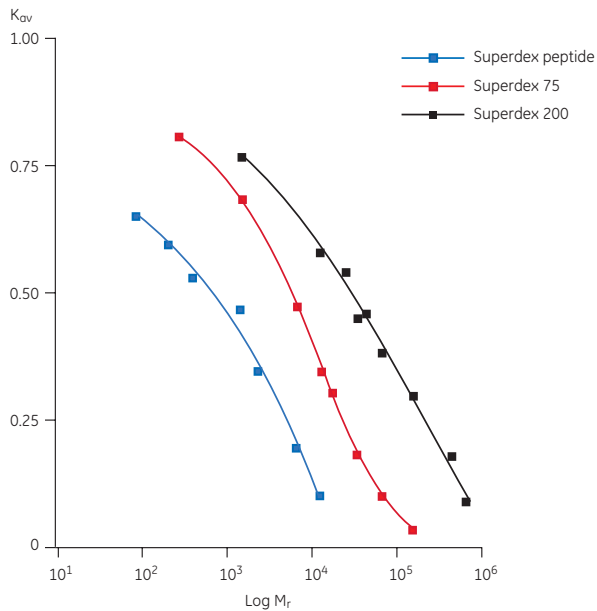


Fig 1.5. Selectivity curves for Superdex.

Selectivity curves are almost linear in the range $K_{av} = 0.1$ to $K_{av} = 0.7$ and can be used to determine the fractionation range of a SEC medium (Fig 1.6).

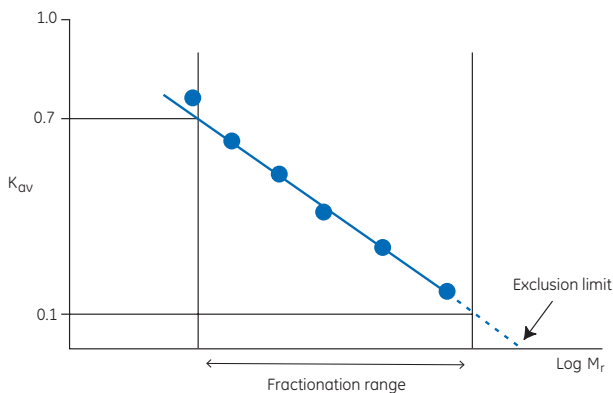


Fig 1.6. Defining fractionation range and exclusion limit from a selectivity curve.

The fractionation range defines the range of molecular weights that have partial access to the pores of the matrix; that is molecules within this range should be separable by high-resolution fractionation. The exclusion limit for a SEC medium, also determined from the selectivity curve, indicates the size of the molecules that are excluded from the pores of the matrix and therefore elute in the void volume.

A steeper selectivity curve means an improved separation of proteins within a smaller fractionation range. Resolution is also affected by band-broadening, which is dependent on the particle size of the medium. The smaller the particle size, the higher the resolution.

An example of the effects of different selectivities between two similar SEC media is shown in Figure 1.7. Superdex 200 Increase and Superose 6 Increase are both media for small-scale preparative purification and analysis, with the same high-flow agarose base matrix (average particle size 8.6 μm). They differ in fractionation ranges, which results in very different chromatography profiles for the same sample mix. Superdex 200 Increase gives excellent resolution for proteins with molecular weight less than 440 000, while the largest protein elutes together with aggregates in the void volume. Superose 6 Increase, on the other hand, has good separation between the largest proteins. The broad peak of IgM was confirmed by light scattering to include different isoforms and aggregates of IgM.

Columns: Superose 6 Increase 10/300 GL and Superdex 200 Increase 10/300 GL
Sample: 1. IgM ($M_r \sim 970\,000$)*, 0.5 mg/ml
2. Thyroglobulin ($M_r\,669\,000$), 1 mg/ml
3. Ferritin ($M_r\,440\,000$), 0.1 mg/ml
4. Bovine serum albumin (BSA, $M_r\,66\,000$), 1 mg/ml
5. Myoglobin ($M_r\,17\,000$), 0.5 mg/ml
6. Vitamin B₁₂ ($M_r\,1355$), 0.05 mg/ml
Sample volume: 100 μl
Flow rate: 0.5 ml/min
Buffer: PBS, (10 mM phosphate buffer, 140 mM sodium chloride, pH 7.4)
System: ÄKTAmicro

* In addition, this sample also contained aggregated forms of IgM.

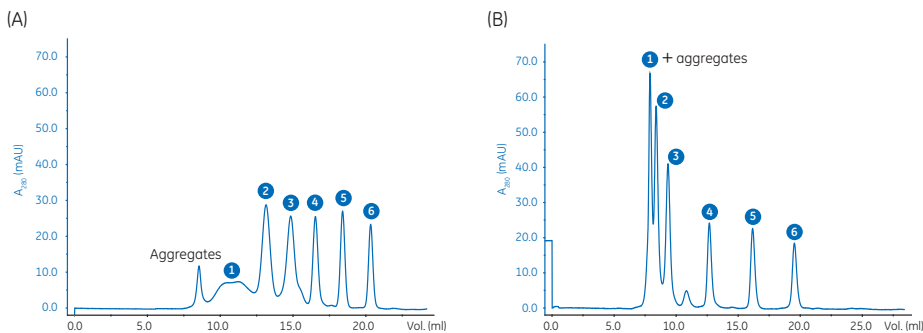


Fig 1.7. Chromatograms showing high-resolution SEC of six standard proteins on (A) Superose 6 Increase 10/300 GL and (B) Superdex 200 Increase 10/300 GL.



When choosing a medium, consider two main factors:

1. The aim of the experiment (high-resolution fractionation or group separation).
2. The molecular weights of the target proteins and contaminants to be separated.

The final scale of purification should also be considered. Figure 1.8 gives some guidance to media selection. Almost all media are available in prepacked columns, which is recommended if you have little experience in column packing.

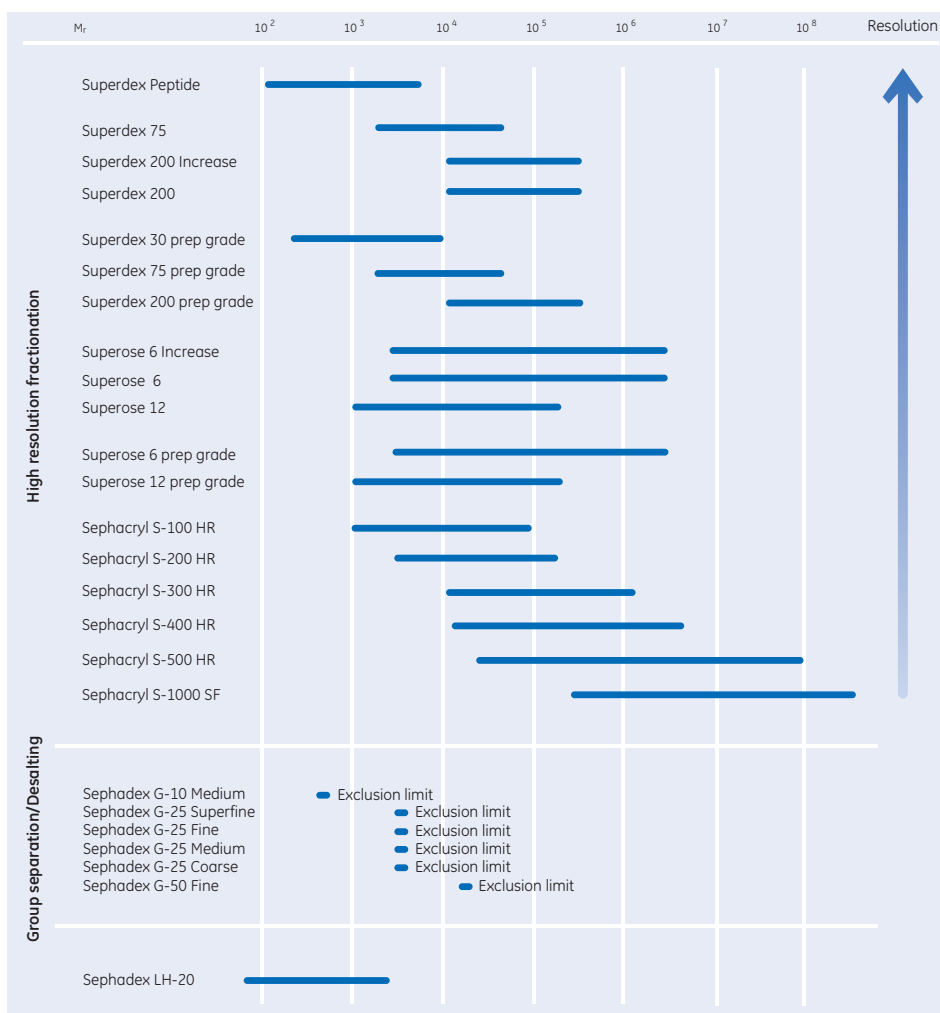


Fig 1.8. SEC media fractionation ranges.



Superdex Increase or Superdex are designed for high resolution, short run times, and high recovery.



Superdex prep grade and Sephacryl are suitable for fast, high-recovery separations at laboratory and industrial scale.

Superdex, Superose, and Sephacryl are high-resolution media with a wide variety of fractionation ranges. In cases when two media have similar fractionation ranges, select the medium with the steepest selectivity curve (see Chapters 2, 3, and 4 for the respective medium) for optimal resolution of all the sample components. If a specific component is of interest, select the medium where the log of molecular weight for the target component falls in the middle of the selectivity curve.



Sephadex is recommended for rapid group separations such as desalting and buffer exchange. Sephadex is used at laboratory and production scale, before, between or after other chromatography purification steps.



For group separations, select SEC media that elute high molecular weight-molecules at the void volume to minimize peak broadening or dilution and reduce time in the column. The lowest molecular weight substances should appear by the time one column volume of buffer has passed through the column.

Table 1.2. Sephadex media properties

Medium	Cut-off	Application examples
Sephadex G-10	700	Desalting of peptides
Sephadex G-25	5000	Desalting of proteins and oligonucleotides
Sephadex G-50	30 000	Removal of free labels from labeled macromolecules

Sample and buffer preparation

Removal of particles in the sample is extremely important for SEC. Clarifying a sample before applying it to a column will avoid the risk of blockage, reduce the need for stringent washing procedures and extend the life of the medium.



Samples must be clear and free from particulate matter, especially when working with bead sizes of 34 μm or less.



Appendix 3 contains an overview of sample preparation techniques. For small sample volumes, a syringe-tip filter of cellulose acetate or polyvinylidene fluoride (PVDF) can be sufficient.

Sample buffer composition

The pH, ionic strength, and composition of the sample buffer will not significantly affect resolution as long as these parameters do not alter the size or stability of the proteins to be separated and are not outside the stability range of the SEC medium. The sample does not have to be in exactly the same buffer as that used to equilibrate and run through the column. Sample is exchanged into the running buffer during the separation, an added benefit of SEC.

Sample concentration and viscosity

SEC is independent of sample mass and hence sample concentration, as can be seen in Figure 1.9. High resolution can be maintained despite high sample concentration and, with the appropriate medium, high flow rates.

Column: XK 16/70 (140 ml)
 Medium: Superdex 200 prep grade
 Sample: Solution of transferrin (M_r 81 000) and IgG (M_r 160 000) by equal weight
 Sample volume: $0.8\% \times V_t$
 Buffer: 50 mM sodium phosphate, 100 mM sodium chloride, pH 7.2
 Flow rate: 1 ml/min (30 cm/h)

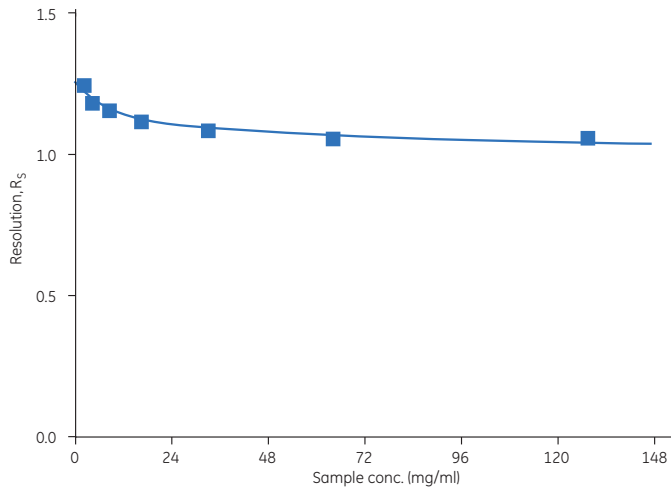


Fig 1.9. Influence of sample concentration on the resolution of transferrin and IgG on Superdex 200 prep grade.

The solubility or the viscosity of the sample might, however, limit the concentration that can be used. A critical variable is the viscosity of the sample relative to the running buffer, as shown by the change in elution profiles of hemoglobin and sodium chloride at different sample viscosities in Figure 1.10.

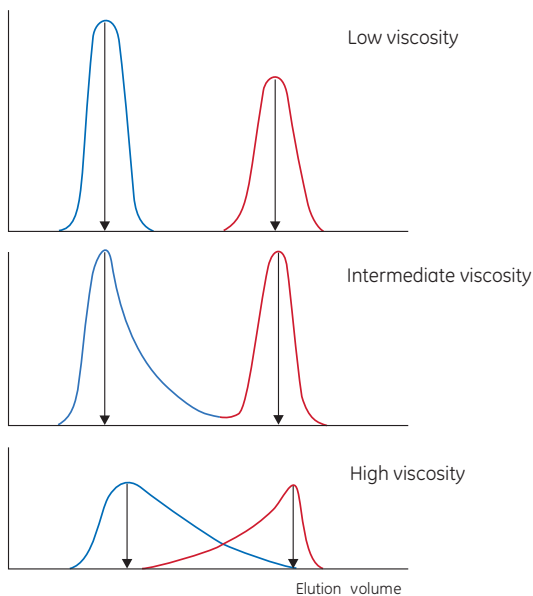


Fig 1.10. Deteriorating separation caused by increasing viscosity. Elution diagrams obtained when hemoglobin (blue) and sodium chloride (red) were separated. Experimental conditions were identical except that the viscosities were altered by the addition of increasing amounts of dextran.



High sample viscosity causes instability of the separation and an irregular flow pattern. This leads to very broad and skewed peaks, and the back pressure might increase.



Samples should generally not exceed 70 mg/ml protein. Dilute viscous samples, but not more than necessary to keep the sample volume low. Remember that viscosity varies with temperature.

Sample volume

Sample volume is one of the most important parameters in SEC. Refer to *Sample volume and column dimensions* earlier in this chapter for more information.

Buffer composition

Buffer composition will generally not directly influence the resolution unless the buffer affects the shape or biological activity of the molecules. Extremes of pH and ionic strength and the presence of denaturing agents or detergents can cause conformational changes, dissociation or association of protein complexes.

Select buffer conditions that are compatible with protein stability and activity. The product of interest will be collected in this buffer. Use a buffer concentration that maintains buffering capacity and constant pH. Use up to 300 mM sodium chloride to avoid nonspecific ionic interactions with the matrix which can be seen as delays in peak elution. Note that some proteins can precipitate in low ionic strength solutions. Volatile buffers such as ammonium acetate or ammonium bicarbonate should be used if the separated product will be lyophilized.



Use high-quality water and chemicals. Solutions should be filtered through 0.45 μm or 0.22 μm filters before use. It is essential to degas buffers before any SEC separation since air bubbles can significantly affect performance. Buffers will be automatically degassed if they are filtered under vacuum.



Choose buffer conditions suitable for protein stability and activity. An increase of sodium chloride concentration up to 300 mM or addition of additives, such as detergent or organic solvents, can improve the result. See further denaturing (chaotropic) agents and detergents, below, and instructions for the product.



When working with a new sample, try these conditions first: 50 mM sodium phosphate, 150 mM sodium chloride, pH 7.0 or select the buffer into which the product should be eluted for the next step (e.g., further purification, analysis, or storage).



Avoid extreme changes in pH or other conditions that can cause inactivation or even precipitation. If the sample precipitates in the SEC column, the column will be blocked, possibly irreversibly, and the sample might be lost.

Denaturing (chaotropic) agents and detergents

Denaturing agents such as guanidine hydrochloride or urea can be used for initial solubilization of a sample as well as in SEC buffers to maintain solubility. However, since the proteins will denature, chaotropics should be avoided unless denaturation is specifically desired.

Superdex and Sephacryl are in general more suitable than classical media such as Sepharose™ or Sephadex for working under dissociating or denaturing conditions or at extreme pH values.

Detergents are useful as solubilizing agents for proteins with low aqueous solubility, such as membrane components, and will not affect the separation. Sometimes, denaturing agents or detergents are necessary to maintain the solubility of the sample. Such additives must be present all the time, both in the running buffer and the sample buffer.



If high concentrations of additives are needed, use lower flow rates to avoid excessive pressure since they can increase the viscosity of the buffer.

If proteins precipitate, elute later than expected, or are poorly resolved during SEC, add a suitable concentration of a denaturing agent or detergent to the running buffer.



Urea or guanidine hydrochloride is very useful for molecular weight determination. The presence of these denaturing agents in the running buffer maintains proteins and polypeptides in an extended configuration. For accurate molecular weight determination the calibration standards must also be run in the same buffer.



Note that selectivity curves are usually determined using globular proteins and do not reflect the behavior of denatured samples.



SEC can be used to exchange the detergent environment of a protein. For example, a protein solubilized in sodium dodecyl sulfate (SDS) could be transferred to a milder detergent such as Triton™ X-100 without losing solubility.

Column and media preparation

To perform a separation, SEC medium is packed into a column between 300 and 600 mm in height for high-resolution fractionation and up to 100 mm in height for group separations. Rapid screening experiments can be performed on 150 mm columns. The volume of the packed bed is determined by the sample volumes that will be applied.

Efficient column packing is essential, particularly for high-resolution fractionation. The efficiency of a packed column defines its ability to produce narrow symmetrical peaks during elution. Column efficiency is particularly important in SEC in which separation takes place as only a single column volume of buffer passes through the column. The uniformity of the packed bed and the particles influences the uniformity of the flow profile and hence affects the shape and width of the peaks. High-performance SEC media with high bed uniformity (smaller and more uniform particles) give decreased peak widths and improved resolution.

Efficiency is defined in terms of theoretical plates per meter (N/m).

$$N/m = 5.54 (V_e/W_{1/2})^2/L$$

where

V_e = peak elution (retention) volume

$W_{1/2}$ = peak width at half peak height

L = bed height (m)

V_e and $W_{1/2}$ are in same units

Refer to Chapter 7, *Size exclusion chromatography in theory* and Appendix 1 for further information on column efficiency and column packing.



Always perform a column efficiency test before first-time use of a column (see Appendix 1). The value from the test should be used as the baseline for the column performance. Note that the result for column efficiency is dependent on the system used, including the capillaries and dead volumes. This means that the column efficiency given in the specification for the column (tested on another system) will not be the same as your initial column efficiency result.



Prepacked columns are highly recommended for optimal performance and reproducible results.



Efficiency can be improved by using a smaller particle size. However, using a smaller particle size can create an increase in back pressure so that flow rate must be decreased and run time extended.



Buffers, media, or prepacked columns must have the same temperature before use. Rapid changes in temperature, for example removing packed columns from a cold room and applying buffer at room temperature, can cause air bubbles in the packing and affect the separation.

Storage solutions and preservatives should be washed away thoroughly before using any SEC medium. Equilibrate the column with 1 to 2 column volumes (CV) of buffer before starting a separation.

Setting column pressure limits

Pressure is generated by the flow through the chromatographic system. For optimal chromatography functionality, it is important to understand the principle of the pressure drop over the different parts of a system (Fig 1.11).

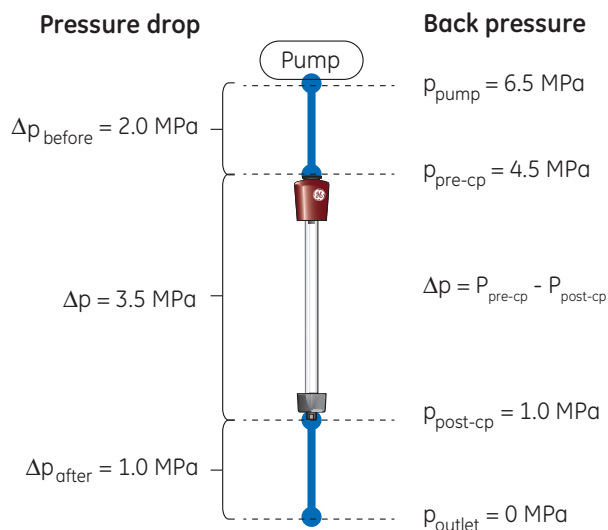


Fig 1.11. Example of the pressure in different parts of a system during run of a column. Note that the pressure values are only used to illustrate the principle.



Δp_{before} does not affect the column.



The pressure on the column hardware is the sum of Δp_{after} and Δp . Do not exceed the column hardware limit!



Δp is individual and needs to be determined for each column.

For more information, refer to the *ÄKTA™ Laboratory-scale Chromatography Systems Instrument Management Handbook*, 29-0108-31.

To protect the column hardware and the packed bed of the chromatographic medium, it is important to set limits that must not be exceeded during the run. There are two important pressure limits that must be taken into consideration:

1. **To protect the column hardware:** Column hardware pressure limit (Fig 1.12), which is the maximum pressure the hardware can withstand without being damaged. This value is fixed for each column type. Leakage from the column could be a sign of excessive pressure on the column hardware.

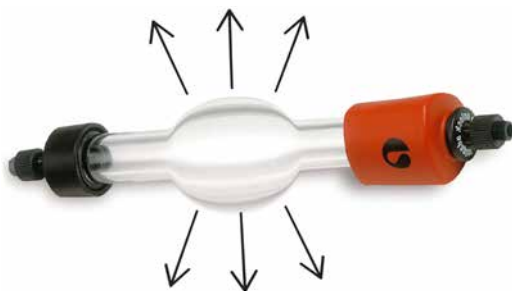


Fig 1.12. Column hardware pressure limit is the maximum pressure the column can withstand without damage.

The column hardware pressure limit is included in the instructions and in UNICORN™ column list for each column type, respectively.

2. **To protect the packed bed:** Delta pressure (Δp) or maximum pressure over the packed bed is the maximum pressure the packed bed of chromatography medium can withstand without risking gap formation (Fig 1.13) or bed collapse. This value varies depending on conditions. A typical value for Δp or maximum pressure drop over the packed bed is provided for each column type in the instructions and UNICORN column list. Note however that Δp is individual for each column and needs to be determined. The procedure for doing this is described in Instructions 29-0272-71. The packed bed is best protected by controlling the flow rate. Use lower flow rates for high-viscosity solutions and/or low temperature (Table 1.3).

Table 1.3. Example of flow rate limits at different viscosity and temperature, Superose 6 Increase 10/300 GL

Temperature	Flow rate (ml/min)	
20°C to 25°C	Maximum flow rate, water	1.5
	Maximum flow rate, 20% ethanol	0.75
4°C to 8°C	Maximum flow rate, water	0.75
	Maximum flow rate, 20% ethanol	0.35



Fig 1.13. The maximum pressure over the packed bed is the maximum pressure the packed bed of chromatography medium can withstand without gap formation. This is not a fixed value.

The pressure over the packed bed is depending on a lot of parameters including:

- Flow rate
- Viscosity of sample and eluent
- Running temperature
- Chromatography medium particle properties
- Column packing

Sample application

A liquid chromatography system should be used for high-resolution separation. For group separations it is possible to use manual purification. Samples can be applied by gravity feed to prepacked columns such as PD-10 Desalting.

Elution and flow rates

Samples are eluted isocratically from a SEC column, using a single buffer system. After sample application the entire separation takes place as one column volume of buffer (equivalent to the volume of the packed bed) passes through the column.

The goal for any separation is to achieve the highest possible resolution in the shortest possible time. Figures 1.14 to 1.16 show that resolution decreases as flow rate increases. Each separation must be optimized to provide balance between these two parameters. Put simply, maximum resolution is obtained with a long column and a low flow rate whereas the fastest run is obtained with a short column and a high flow rate. Suitable flow rates for high-resolution fractionation or group separation are supplied with each product.

The advantage of a higher flow rate (and consequently a faster separation) outweighs the loss of resolution in the separation in certain circumstances.

Column: Superdex 200 Increase 3.2/300
Sample: 1. Thyroglobulin (M_r 669 000), 3 mg/ml
2. Ferritin (M_r 440 000), 0.3 mg/ml
3. Aldolase (M_r 158 000), 3 mg/ml
4. Conalbumin (M_r 75 000), 3 mg/ml
5. Ovalbumin (M_r 44 000), 3 mg/ml
6. Carbonic anhydrase (M_r 29 000), 3 mg/ml
7. Ribonuclease A (M_r 13 700), 3 mg/ml
Sample volume: 10 μ l
Buffer: 10 mM sodium phosphate, 140 mM sodium chloride, pH 7.4
Flow rate: 0.15 and 0.025 ml/min, room temperature
System: ÄKTApurifier

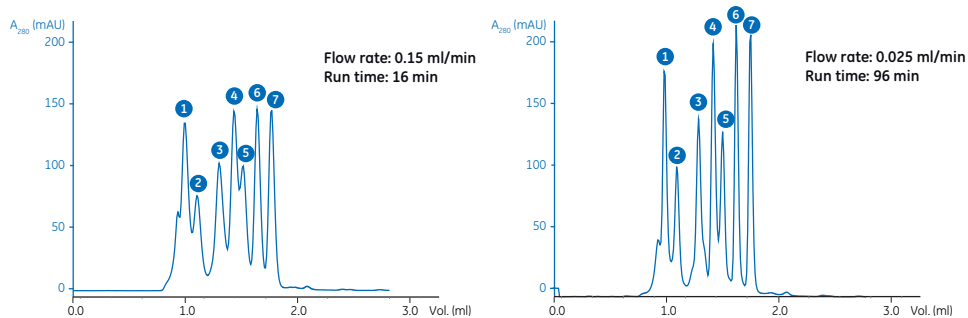


Fig 1.14. Comparison of protein separation on Superdex 200 Increase 3.2/300 at different flow rates.

Column: HiLoad 16/600 Superdex 30 prep grade
 Sample: Insulin-like growth factor 1 (IGF-1) containing monomers and dimers
 Sample load: 1 ml ($0.8\% \times V_t$)
 Sample concentration: (A) 1.25 mg/ml
 (B) 5 mg/ml
 Buffer: 50 mM sodium acetate, 100 mM sodium chloride, pH 5.0
 Flow rates: 15 to 80 cm/h

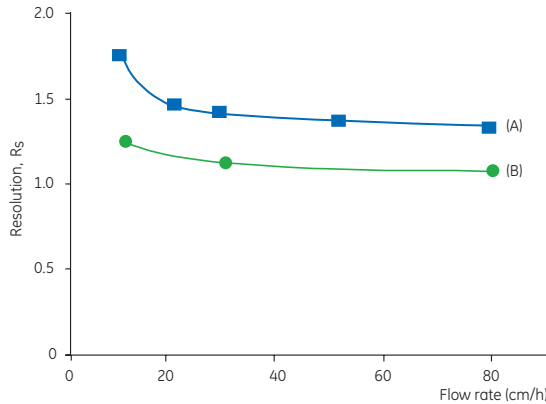


Fig 1.15. Resolution between (A) 1.25 mg/ml and (B) 5 mg/ml concentrations of IGF-1 containing monomers and dimers at different flow rates.

Columns: HiPrep 16/10 Sephacryl S-100 HR
 HiPrep 16/10 Sephacryl S-200 HR
 HiPrep 16/10 Sephacryl S-300 HR
 Sample: IgG, ovalbumin, cytochrome C, 1:2:1
 Sample load: 2.4 ml ($2\% \times V_t$)
 Total sample load: 8 mg
 Buffer: 50 mM sodium phosphate, 150 mM sodium chloride, 0.02% sodium azide, pH 7.0

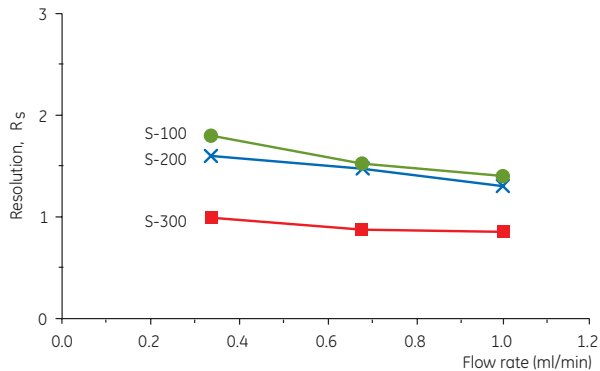


Fig 1.16. Influence on resolution between IgG, ovalbumin, and cytochrome C using different SEC media, at different flow rates.



If peaks are well separated at a low flow rate, increase the flow rate or use a shorter column if possible to save time. Alternatively, increase the sample volume and benefit from a higher capacity without significant loss of resolution.

For group separations such as desalting, monitor the elution of protein at A_{280} and follow the elution of the salt peak using a conductivity monitor. Adjust flow rate and sample volume to balance speed of separation against an acceptable level of salt in the final sample. Recommended flow rates are given in the instructions supplied with each product.





Flow rate is measured in volume terms, for example ml/min, but when comparing results between columns of different sizes it is useful to use the linear flow, cm/h. A conversion table is available in Appendix 5. Results obtained at the same linear flow on different sized columns will be comparable as far as the effects of flow rate are concerned.

Selecting a smaller particle size of the same medium (if available) can also help to achieve the correct balance between flow rate and resolution. Smaller particles of the same medium can increase column efficiency, and improve resolution to allow the use of higher flow rates. However, smaller particles can also result in increased back pressure and this factor can become restrictive if the intention is to scale up the separation.

Include a wash step at the end of a run to remove any molecules that have been retained on the column, to prevent cross-contamination and to prepare the column for a new separation.

Controlling flow rates

Accurate, reproducible control of the flow rate is not only essential for good resolution, but also for reliability in routine preparative work and repeated experiments.

-  Use a chromatography system (rather than a peristaltic pump or gravity feed) to fully utilize the high rigidity and excellent flow properties of Sephacryl, Superose, or Superdex for high-resolution fractionation.
-  Always pump the buffer to a column rather than drawing the buffer through the column with the pump below. This reduces the risk of bubble formation as a result of suction. If you have packed the column yourself, always use a lower flow rate for separation than the flow rate used for column packing.
-  Use a syringe or a pump for work with small prepacked columns such as HiTrap Desalting. Gravity feed with PD-10 Desalting for group separations of small sample volumes.
-  SEC columns must not run dry. Ensure that there is sufficient buffer for long, unattended runs or that the pump is programmed to stop the flow after a suitable time. Columns that run dry must be repacked since the packed bed has been destroyed.


Method development for high-resolution fractionation

Prepacked columns are delivered with recommended running conditions that give satisfactory results in most situations. If optimization is needed, follow these steps (given in order of priority):

1. Select the medium that will give optimal resolution of the target protein(s), see the SEC media fractionation range guide, Figure 1.8.
2. To ensure reproducibility and high resolution, select a prepacked column that is suited to the volume of sample that needs to be processed (see Chapters 2 to 4 for details of prepacked columns containing Superdex, Superose, or Sephacryl).
3. Select the highest flow rate that maintains resolution and minimizes separation time. Check recommended flow rates supplied in the instructions for the specific medium and column.
4. Determine the maximum sample volume that can be loaded without reducing resolution.

Higher flow rates and viscous buffers give higher operating pressures (remember that buffer viscosity increases when running at 4°C).






The packed bed is protected by the following actions:

- Decreasing the flow rate (Table 1.3).
 - Determining the maximum operating pressure at intended conditions (buffer and temperature). See the section *Setting column pressure limits* earlier in this chapter.
-  If greater resolution is required, increase the bed height by connecting two columns containing the same medium in series. Alternatively, try a medium with the same or similar fractionation range, but with a smaller particle size.

To process larger sample volumes, see scaling up below.

Maintenance of SEC columns

Routine cleaning of the SEC column, for example every 20 runs (depending on sample), is recommended. Cleaning will prolong the column life time and is performed in order to remove any precipitated proteins or other contaminants that can build up on the column. Cleaning is necessary when a colored band can be seen at top of the column, there is loss in resolution, or a significant increase in back pressure. Detailed cleaning procedures for each SEC medium are given in Chapters 2 to 6 and in the instructions for the product.

-  Always use filtered buffers and samples to reduce the need for additional column maintenance. See Appendix 3 for further details on sample preparation.
-  In case of increased back pressure, see also Troubleshooting section in this chapter.
-  Always use well degassed buffers to avoid the formation of air bubbles in the packed column during a run.
-  Buffers and prepacked columns should be kept at the same temperature to prevent air bubbles forming in the column.
-  Filter cleaning solutions before use and always re-equilibrate the column with 2 to 3 CV of buffer before the next separation.

Equipment selection

Appendix 4 provides a guide to the selection of suitable systems for SEC separation.

Scaling up

After establishing a high-resolution or group separation on a small column, larger columns can be packed to process larger sample volumes in a single step. General guidelines for scaling up are shown in Table 1.4.

Table 1.4. General guidelines for scaling up SEC separations

Maintain	Increase
Bed height	Column diameter
Linear flow rate	Volumetric flow rate
Sample composition	Sample volume

To scale up a SEC separation, follow this workflow:

1. Optimize the separation at small scale (see previous section in this chapter; *Method development for high-resolution fractionation*).
2. Maintain the sample concentration and the ratio of sample to column volume.
3. Increase the column volume by increasing the cross-sectional area of the column.
4. Maintain the bed height.
5. Run the separation at the same linear flow rate as used on the smaller column (see Appendix 5).

Refer to Appendix 1 for column selection and column packing.

Different factors related to the equipment affect performance after scale-up. If a larger column has a less efficient flow distribution system, or a larger system introduces dead volumes, peak broadening can occur. This will cause extra dilution of the product fraction or even loss of resolution if the application is sensitive to variations in efficiency.

For media such as Superdex or Superose, it is usually recommended to select a larger particle size for scale-up. For high-resolution fractionation, pack a small column containing the larger particles and repeat the separation to facilitate optimization that is needed to achieve the same resolution on the larger column.

Scaling up on Sephadex G-25, even to production scale, is a straightforward and well-established process. Well-known examples of commercial applications include buffer exchange in processes for removing endotoxins from albumin, and preparative steps during the production of vaccines. Figure 1.17 shows an example of a large-scale buffer exchange step used during the production of albumin and IgG from human plasma.

Column: BPSS 400/600, 75 l
Sample: 10 l of human plasma
Buffer: 25 mM sodium acetate
Flow rate: 240 l/h

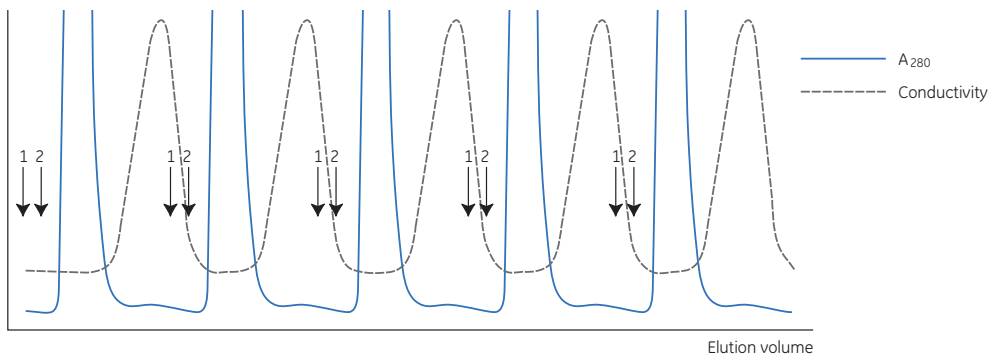


Fig 1.17. Chromatogram of the buffer exchange step on Sephadex G-25 Coarse during production of albumin and IgG from human plasma. 1: sample application; 2: eluent application.

BioProcess™ media for large-scale production

Specific BioProcess media have been designed for each chromatographic stage in a process from capture to polishing. Use BioProcess media for every stage results in a systematic approach to method development. Column packing methods are established for a wide range of scales. The same BioProcess media can be used for development work, pilot studies, and routine production.

High flow rates, high capacity, and high recovery contribute to the overall economy of an industrial process.

All BioProcess media can be cleaned- and sanitized-in-place.


Regulatory Support Files contain details of performance, stability, extractable compounds and analytical methods available. The essential information in these files gives an invaluable starting point for process validation, as well as support for clinical and marketing applications submitted to regulatory authorities.

Large-capacity production integrated with clear ordering and delivery routines mean BioProcess media are available in the right quantity, at the right place, at the right time. Future supplies of BioProcess media are assured, making them a safe investment for long-term production.

BioProcess media are produced following validated methods and are tested under strict control, fulfilling performance specifications. A certificate of analysis is available with each order. Our media safety stock agreements offer the right quantity of media, manufactured to specified quality levels, and delivered at the right time.


Troubleshooting

This section focuses on practical problems that can occur during SEC. Figure 1.18 indicates how the trace of the a chromatogram can deviate from normal during a separation. Table 1.5 on the following pages contains suggestions of possible causes and their remedies.

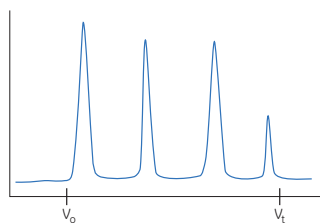


Satisfactory separation

Well-resolved, symmetrical peaks.

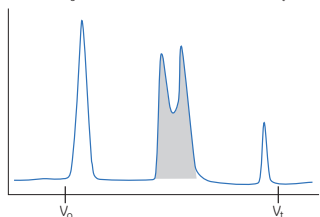


Poor resolution

Review factors affecting resolution, including media selection, particle size, sample volume: column volume, and flow rate.

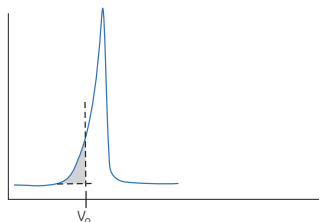


Leading peaks

Asymmetric peaks: sample elutes before void volume indicates channeling in the column bed. Leading peaks can also be due an overpacked column (packed at too high a pressure or flow rate). The column might need to be repacked.

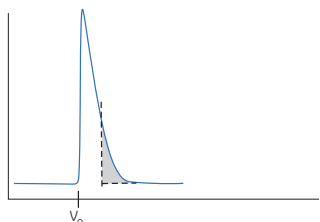

Tailing peaks

Asymmetric peaks: sample application uneven. Check the top of column if possible. Ensure the medium is evenly packed and that sample is applied without disturbing the packed bed. Tailing peaks can also be due to underpacking of the column (packed at too low a pressure or flow rate).

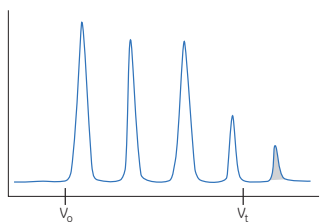

Late elution

Peaks seen after one column volume of buffer has passed through the column. Always include a wash step between runs to ensure removal of late eluting molecules.

Fig 1.18. Normal chromatograms and chromatograms deviating from normal behavior.

Table 1.5. Troubleshooting guide for SEC

Situation	Cause	Remedy
Peak of interest is poorly resolved from other major peaks.	Sample volume is too high.	Decrease sample volume and apply sample carefully.
	Sample is too viscous.	Dilute with buffer, but check maximum sample volume. Maintain protein concentration below 70 mg/ml.
	Sample contains particles.	Re-equilibrate column, filter sample, and repeat.
	Column not mounted vertically.	Adjust column position. Column might need to be repacked.
	Column is poorly packed.	Check column efficiency (see Appendix 1). Repack if needed*. Use prepacked columns.
	Column is dirty.	Clean and re-equilibrate.
	Incorrect medium.	Check selectivity curve. Check for adsorption effects. Consider effects of denaturing agents or detergents if present.
	Large dead volumes.	Minimize dead volumes in tubings and connections.
Protein does not elute as expected.	Column is too short.	See Appendix 1 for recommended bed heights.
	Flow rate is too high.	Check recommended flow rates. Reduce flow rate.
	Ionic interactions between protein and matrix.	Maintain ionic strength of buffers above 50 mM (preferably include up to 300 mM sodium chloride).
	Hydrophobic interactions between protein and matrix.	Reduce salt concentration to minimize hydrophobic interaction. Increase pH. Add suitable detergent or organic solvent, e.g., 5% isopropanol.
	Sample has not been filtered properly.	Clean the column, filter the sample, and repeat.
	Sample has changed during storage.	Prepare fresh samples.
	Column is not equilibrated sufficiently.	Repeat or prolong the equilibration step.
	Proteins or lipids have precipitated on the column.	Clean the column or use a new column.
Protein elutes later than expected or even after running a total column volume.	Column is overloaded with sample.	Decrease the sample load.
	Microbial growth has occurred in the column.	Microbial growth rarely occurs in columns during use. To prevent infection of packed columns, store in 20% ethanol when possible.
Protein elutes later than expected or even after running a total column volume.	Hydrophobic and/or ionic interactions between protein and matrix.	Reduce salt concentration to minimize hydrophobic interaction. Increase pH. Add suitable detergent or organic solvent, e.g., 5% isopropanol.
		Increase salt concentration (up to 300 mM) to minimize ionic interaction.
Peaks elute late and are very broad.	Column is dirty.	Clean and re-equilibrate.
Protein elutes earlier than expected (before the void volume).	Channeling in the column.	Repack column using thinner slurry of medium. Avoid introduction of air bubbles*.
Molecular weight or shape is not as expected.	Protein has changed during storage.	Prepare fresh samples.
	Ionic interactions between proteins and matrix.	Maintain ionic strength of buffers above 50 mM (preferably include 150 mM sodium chloride).
	Hydrophobic interactions between protein and matrix.	Reduce salt concentration to minimize hydrophobic interaction. Increase pH. Add suitable detergent or organic solvent, e.g., 5% isopropanol.
	Precipitation of protein in the column filter and/or at the top of the bed.	If possible, clean the column, exchange or clean the filter or use a new column.
Leading or very rounded peaks in chromatogram.	Column overloaded.	Decrease sample load and repeat.
Tailing peaks.	Column is 'under packed'.	Check column efficiency (see Appendix 1). Repack using a higher flow rate. Use prepacked columns*.

Situation	Cause	Remedy
Obtained column efficiency is not the same as in the column specification.	Result for column efficiency is dependent on the system and cannot be expected to be the same.	Use the obtained column efficiency for later comparisons in order to detect any changes in column performance.
Leading peaks.	Column is over packed.	Check column efficiency (see Appendix 1). Repack using a lower flow rate. Use prepacked columns*.
Medium/beads appear in eluent.	Bed support end piece is loose or broken.	Replace or tighten.
	Column operated at too high pressure.	Do not exceed recommended operating pressure for medium or column.
Low recovery of activity but normal recovery of protein.	Protein is unstable or inactive in the buffer.	Determine the pH and salt stability of the protein.
	Enzyme separated from cofactor or similar.	Test by pooling aliquots from the reactions and repeat the assay.
Results are not reproducible.	The new column is not saturated by protein in the first two to three runs.	Perform test runs until the column is saturated with protein and stability is obtained.
Lower yield than expected.	Protein has been degraded by proteases.	Add protease inhibitors to the sample and buffers to prevent proteolytic digestion. Run sample through a medium such as Benzamidine 4 Fast Flow (high sub) to remove trypsin-like serine proteases.
	Adsorption to filter during sample preparation.	Use another type of filter.
	Sample precipitates.	Can be caused by removal of salts or unsuitable buffer conditions.
	Hydrophobic proteins.	Use denaturing agents, polarity reducing agents, or detergents.
	Nonspecific adsorption.	Increase salt concentration in the buffer, up to 300 mM sodium chloride.
More sample is recovered than expected.	Protein is coeluting with other substances.	Optimize conditions to improve resolution. Check buffer conditions used for assay before and after the run. Check selection of medium.
More activity is recovered than was applied to the column.	Different assay conditions have been used before and after the chromatography step.	Use the same assay conditions for all the assays in the purification scheme.
Reduced or poor flow through the column.	Presence of lipoproteins or protein aggregates.	Remove lipoproteins and aggregates during sample preparation (see Appendix 3).
	Protein precipitation in the column caused by removal of stabilizing agents during separation.	Modify the eluent to maintain stability.
	Blocked column filter.	If possible, replace the filter or use a new column. Always filter samples and buffer before use.
	Blocked end-piece, adapter, or tubing.	If possible, remove and clean or use a new column.
	Precipitated proteins.	Clean the column using recommended methods or use a new column.
	Bed compressed.	If possible, repack the column or use a new column*.
	Microbial growth.	Microbial growth rarely occurs in columns during use. To prevent infection of packed columns, store in 20% ethanol when possible.
	Fines (Sephadex).	Decant fines before column packing. Avoid using magnetic stirrers that can break the particles.

Situation	Cause	Remedy
Back pressure increases during a run or during successive runs.	Turbid sample.	Improve sample preparation (see Appendix 3). Improve sample solubility by the addition of ethylene glycol, detergents, or organic solvents.
	Precipitation of protein in the column filter and/or at the top of the bed.	Clean using recommended methods. If possible, exchange or clean filter or use a new column. Include any additives that were used for initial sample solubilization in the running buffer.
	Clogged on-line filters.	Exchange on-line filters.
Air bubbles in the bed.	Column packed or stored at cool temperature and then warmed up.	Note that small amounts of air will normally not affect the performance of the column. Remove air bubbles by passing degassed buffer in an up-flow direction at low flow rate. Note that reverse flow should not be used for Sephacryl columns. Take special care if buffers are used after storage in a fridge or cold-room. Do not allow column to warm up due to sunshine or heating system. Repack column if possible (see Appendix 1*).
	Buffers not properly degassed.	Buffers must be degassed thoroughly.
Space between medium bed and adapter.	Back pressure increase or bed insufficiently packed.	Turn down the adapter to the medium bed. Perform a column performance control.
Cracks in the bed.	Large air leak in column.	Check all connections for leaks. Repack the column if possible (see Appendix 1).
Distorted bands as sample runs into the bed.	Air bubble at the top of the column or in the inlet adapter.	If possible, re-install the adapter taking care to avoid air bubbles. Perform a column performance control.
	Particles in buffer or sample.	Filter or centrifuge the sample. Protect buffers from dust.
	Blocked or damaged net in upper adapter.	If possible, dismantle the adapter, clean or replace the net. Keep particles out of samples and eluents.
Distorted bands as sample passes down the bed.	Column poorly packed.	Suspension too thick or too thin. Bed packed at a temperature different from run.
		Bed insufficiently packed (too low packing pressure, too short equilibration). Column packed at too high pressure.

* Not all prepacked columns can be repacked.

Chapter 2

Superdex: for high resolution, short run times, and high recovery

Superdex are SEC media consisting of a composite base matrix of dextran and agarose (Fig 2.1). This matrix combines the excellent SEC properties of cross-linked dextran with the physical and chemical stabilities of highly cross-linked agarose, to produce a separation medium with outstanding selectivity and high resolution. In addition, its low nonspecific interaction permits high recovery of biological material. Together these properties make Superdex an excellent choice for all applications from laboratory to process scale.

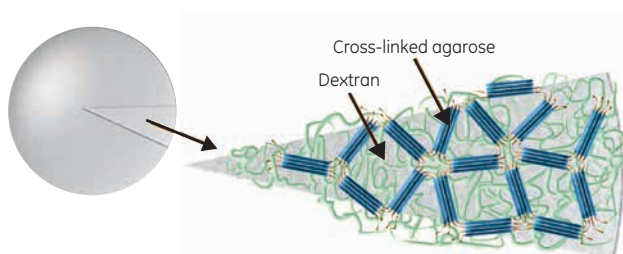


Fig 2.1. A schematic section of a Superdex particle. In Superdex, the dextran chains are covalently linked to a highly cross-linked agarose matrix.

Superdex Increase is the next generation Superdex medium and has improved performance even further by providing increased resolution and shorter run times. This is achieved by using a high-flow agarose base matrix, which has higher flow/pressure tolerance, smaller bead size, and narrower particle size distribution. Figure 2.2 shows the fractionation ranges for all variants of Superdex media.

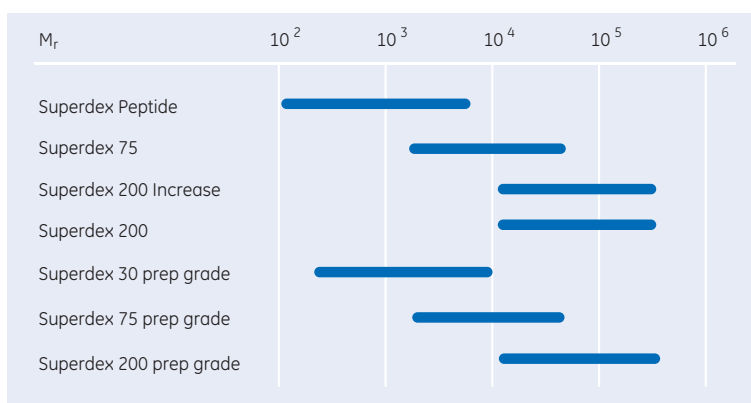


Fig 2.2. Fractionation ranges for Superdex.

One of the common properties of Superdex media is the high rigidity that allows even viscous eluents, such as urea, to be run at relatively high flow rates. Also, nonspecific interactions are negligible under normal chromatography conditions when using buffers with ionic strengths in the range 0.15 M to 1.5 M. For cleaning-in-place, up to 1 M sodium hydroxide can be used since the media are alkali tolerant.

Three types of Superdex are available: Superdex Increase, Superdex, and Superdex prep grade.

Superdex Increase

Superdex 200 Increase (average particle size 8.6 µm) is the next generation SEC medium. It is designed for high resolution and short run times, resulting in exceptional analytical results and high purity. Superdex 200 Increase has a broad fractionation range that allows separation of a large variety of proteins (M_r 10 000 to 600 000) with an optimized resolution for the antibody molecular weight range of M_r 100 000 to 300 000.

In comparison with Superdex 200, Superdex 200 Increase offers increased resolution and shorter run time (Fig 2.3). The improved performance is due to the combination of more rigid and smaller beads with narrower particle size distribution.

Columns:	Superdex 200 Increase 10/300 GL and Superdex 200 10/300 GL
Sample:	1. Thyroglobulin (M _r 669 000), 3 mg/ml 2. Ferritin (M _r 440 000), 0.3 mg/ml 3. Aldolase (M _r 158 000), 3 mg/ml 4. Conalbumin (M _r 75 000), 3 mg/ml 5. Ovalbumin (M _r 44 000), 3 mg/ml 6. Carbonic anhydrase (M _r 29 000), 3 mg/ml 7. RNase (M _r 13 700), 3 mg/ml
Sample volume:	100 µl
Buffer:	10 mM sodium phosphate, 140 mM sodium chloride, pH 7.4
Flow rate:	1 ml/min (Superdex 200 Increase) and 0.5 ml/min (Superdex 200)
System:	ÅKTApurifier

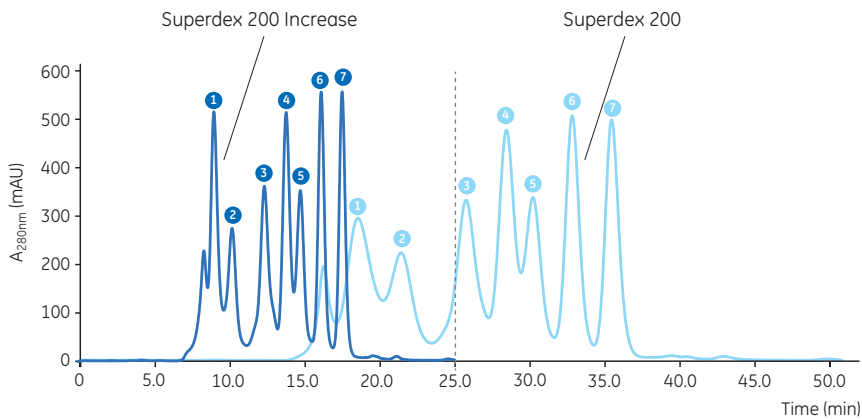


Fig 2.3. Comparison between Superdex 200 Increase and Superdex 200 (both in 10/300 GL column). Higher resolution and shorter run time is obtained using Superdex 200 Increase.

Superdex 200 Increase is agarose-based and, unlike silica-based media which decompose at high pH, it can be cleaned using sodium hydroxide. Cleaning with sodium hydroxide is highly efficient and prolongs column life and minimizes the risk for carry-over between different runs. The selectivity curve for Superdex 200 Increase is shown in Figure 2.4.

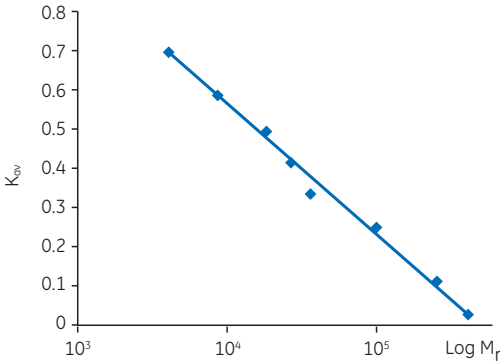


Fig 2.4. Superdex 200 Increase selectivity curve for proteins.

Superdex 200 Increase is available in different column formats, which gives versatility for different application purposes, such as rapid screening, small-scale preparative purification, as well as high-resolution analysis (Table 2.1).

Table 2.1. Selecting Superdex 200 Increase columns

Type of application/column	10/300 GL	5/150 GL	3.2/300
Small-scale preparative runs (mg)	×		
High-resolution analysis (25 to 500 µl)	×		
Purity check		×	
Rapid screening When time is limited and low buffer and sample consumption is important		×	
Small-scale preparative runs (µg) When sample amount is limited and low consumption of buffer is important			×
High-resolution analysis (4 to 25 µl) When sample amount is limited and low consumption of buffer is important			×

Superdex

Superdex Peptide, Superdex 75, and Superdex 200 have an average bead size of 13 μm and are designed for different fractionation ranges. The media are available in prepacked columns for high performance. Superdex Peptide is suitable for high-resolution fractionation of peptides, oligonucleotides, and small proteins (M_r 100 to 7000). Figure 2.5 shows a separation of standard peptides on Superdex Peptide 10/300 GL.

Column:	Superdex Peptide 10/300 GL
Sample:	1. Cytochrome C (M_r 12 384), 1 mg/ml 2. Aprotinin (M_r 6512), 2 mg/ml 3. Vitamin B ₁₂ (M_r 1355) 0.1 mg/ml 4. (Gly) ₃ (M_r 189), 0.1 mg/ml 5. Gly (M_r 75), 7.8 mg/ml
Sample load:	50 μl
Buffer:	50 mM phosphate, 150 mM sodium chloride, pH 7.0
Flow rate:	0.5 ml/min, room temperature

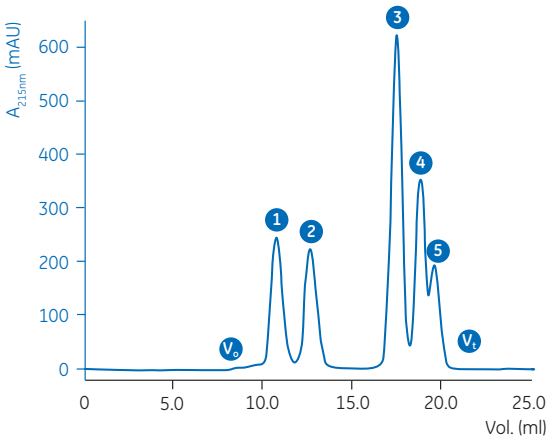


Fig 2.5. Separation of standard peptides on Superdex Peptide 10/300 GL.

Superdex 75 is designed for high-resolution fractionation of biomolecules with M_r 3000 to 70 000, such as recombinant proteins. Examples of application areas are screening of solubilization conditions for membrane proteins, study of protein-protein interactions, and rapid purity check of proteins. A dimer-monomer separation of a recombinant protein is shown in Figure 2.6.

Column: Superdex 75 10/300 GL
 Sample: recombinant Cys-protein
 Sample load: 200 μ l
 Buffer: 50 mM Tris-HCl, 1 mM EDTA, 150 mM sodium chloride, pH 8.4
 Flow rate: 0.5 ml/min

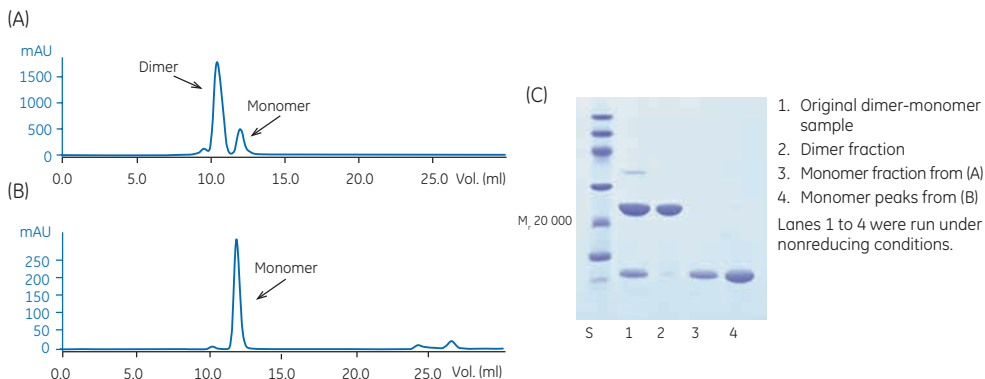


Fig 2.6. (A) Dimer-monomer separation of a recombinant cysteine-containing protein (recombinant Cys-protein) on Superdex 75 10/300 GL. (B) purification of the dimer fraction reduced with DTE. (C) Coomassie™ stained SDS-PAGE gel. Lane S is LMW-SDS Marker Kit (17-0446-01).

Superdex 200 (the predecessor of Superdex 200 Increase) has a broad fractionation range, M_r 10 000 to 600 000, for separation of a large variety of proteins. Use Superdex 200 Increase to give higher resolution and shorter run times compared with Superdex 200.

Superdex prep grade

Superdex prep grade has an average bead size of 34 μ m and is excellent for preparative purification and scale-up purposes. The high stability makes Superdex prep grade suitable for use in larger scale where high flow rates and fast, effective cleaning-in-place (CIP) protocols are required. Since the media can withstand high flow rates during equilibration and cleaning, the overall cycle time can be kept short.

Superdex prep grade is available as Superdex 30 prep grade, Superdex 75 prep grade, and Superdex 200 prep grade for different fractionation ranges (Figure 2.1). Pressure-flow relationship curves for Superdex prep grade and selectivity curves are shown in Figure 2.7 and 2.8, respectively.

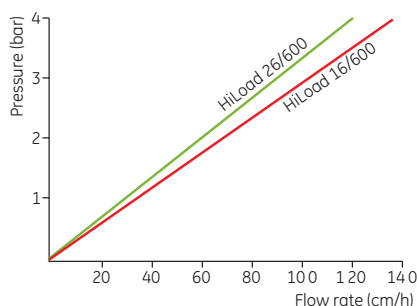


Fig 2.7. Pressure drop as a function of flow rate for HiLoad columns packed with Superdex prep grade. Bed height approximately 60 cm in distilled water at 25°C. To calculate volumetric flow rate, multiply linear flow by cross-sectional area of column (2.0 cm² for XK 16, 5.3 cm² for XK 26). See Appendix 5 for more information about flow rate calculations.

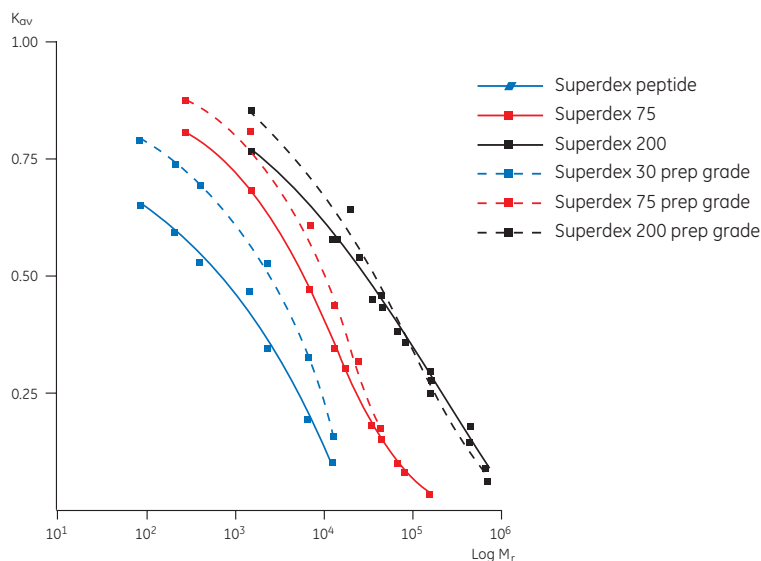


Fig 2.8. Selectivity curves for Superdex (13 μ m) and Superdex prep grade (34 μ m) media.

Superdex prep grade is available preppacked in HiLoad columns and in bulk packs. A comparison of the selectivity of different Superdex prep grade media is shown using standard proteins in Figure 2.9.

Columns: (A) HiLoad 16/600 Superdex 75 prep grade
(B) HiLoad 16/600 Superdex 200 prep grade

Sample: 1. Ferritin (M_r 440 000), 0.24 mg/ml
2. IgG (M_r 158 000), 0.2 mg/ml
3. Albumin (M_r 67 000), 5 mg/ml
4. Ovalbumin (M_r 43 000), 4 mg/ml
5. Myoglobin (M_r 17 000), 1.5 mg/ml

Sample load: 500 μ l

Buffer: 50 mM phosphate buffer, 150 mM sodium chloride, 0.01% sodium azide, pH 7.0

Flow rate: 1.5 ml/min (45 cm/h)

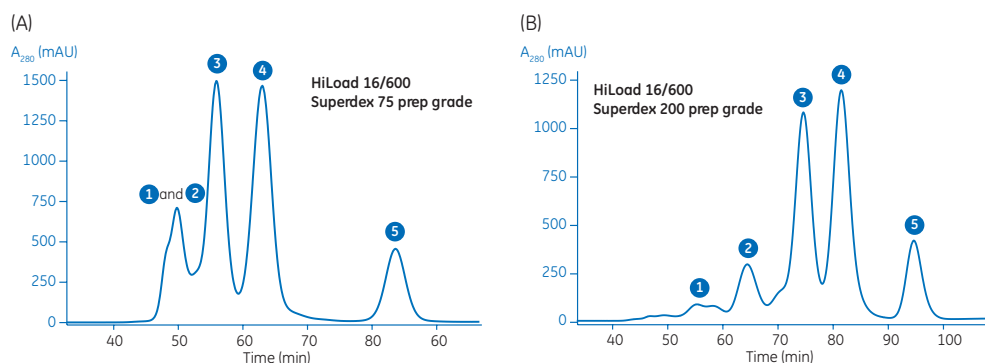


Fig 2.9. Comparison of the selectivity of Superdex 75 prep grade and Superdex 200 prep grade for standard proteins. Superdex 75 prep grade (A) gives excellent resolution of the three proteins in the molecular weight range of 17 000 to 67 000 while the two largest proteins (ferritin and IgG, peaks 1 and 2) elute together in the void volume (V_0). Superdex 200 prep grade (B) resolves the two largest proteins completely, however. The ferritin (peak 1) contains aggregates that result in the observed double peak.

Separation options

Superdex is produced with different average particle sizes and different selectivities (see Table 2.2).



Use the prepacked columns with Superdex Peptide, Superdex 75, and Superdex 200 Increase for small-scale preparative purification and analytical runs.



Use columns prepacked with Superdex 30 prep grade, Superdex 75 prep grade, or Superdex 200 prep grade media for preparative applications.



Use bulk media of Superdex 30 prep grade, Superdex 75 prep grade, and Superdex 200 prep grade for preparative purification with larger sample volumes of up to 13 ml.

Table 2.2. Separation options with Superdex media

Product*	Fractionation range, M_r (globular proteins)	Sample loading capacity†	Maximum pressure drop over the packed bed	Recommended operational flow rate‡
Superdex 200 Increase 3.2/300	1×10^4 to 6×10^5	4 to 50 μ l	3.0 MPa, 30 bar, 435 psi**	0.075 ml/min
Superdex 200 Increase 5/150 GL	1×10^4 to 6×10^5	4 to 50 μ l	3.0 MPa, 30 bar, 435 psi**	0.45 ml/min
Superdex 200 Increase 10/300 GL	1×10^4 to 6×10^5	25 to 500 μ l	3.0 MPa, 30 bar, 435 psi**	0.75 ml/min
Superdex Peptide 3.2/300	1×10^2 to 7×10^3	< 50 μ l	2.0 MPa, 20 bar, 290 psi	0.05 ml/min
Superdex Peptide 10/300 GL	1×10^2 to 7×10^3	25 to 500 μ l	2.0 MPa, 20 bar, 290 psi	< 1.0 ml/min
HiLoad 16/600 Superdex 30 pg [§]	$< 1 \times 10^4$	≤ 5 ml	0.3 MPa, 3 bar, 42 psi	1.0 ml/min
HiLoad 26/600 Superdex 30 pg [§]	$< 1 \times 10^4$	≤ 13 ml	0.3 MPa, 3 bar, 42 psi	2.6 ml/min
Superdex 30 pg [§] (Bulk medium)	$< 1 \times 10^4$	0.5% to 4% of total column volume	Column-dependent	10 to 50 cm/h
Superdex 75 3.2/300	3×10^3 to 7×10^4	< 50 μ l	2.4 MPa, 24 bar, 350 psi	0.05 ml/min
Superdex 75 5/150 GL	3×10^3 to 7×10^4	4 to 50 μ l	1.8 MPa, 18 bar, 260 psi	0.3 ml/min
Superdex 75 10/300 GL	3×10^3 to 7×10^4	25 to 500 μ l	1.8 MPa, 18 bar, 260 psi	0.5 to 0.75 ml/min
HiLoad 16/600 Superdex 75 pg [§]	3×10^3 to 7×10^4	≤ 5 ml	0.3 MPa, 3 bar, 42 psi	1.0 ml/min
HiLoad 26/600 Superdex 75 pg [§]	3×10^3 to 7×10^4	≤ 13 ml	0.3 MPa, 3 bar, 42 psi	2.6 ml/min
Superdex 75 pg [§] (Bulk medium)	3×10^3 to 7×10^4	0.5% to 4% of total column volume	Column-dependent	10 to 50 cm/h
Superdex 200 3.2/300	1×10^4 to 6×10^5	< 50 μ l	1.5 MPa, 15 bar, 220 psi	0.05 ml/min
Superdex 200 5/150 GL	1×10^4 to 6×10^5	4 to 50 μ l	1.5 MPa, 15 bar, 220 psi	0.3 ml/min
Superdex 200 10/300 GL	1×10^4 to 6×10^5	25 to 500 μ l	1.5 MPa, 15 bar, 220 psi	0.5 to 0.75 ml/min
HiLoad 16/600 Superdex 200 pg [§]	1×10^4 to 6×10^5	≤ 5 ml	0.3 MPa, 3 bar, 42 psi	1.0 ml/min
HiLoad 26/600 Superdex 200 pg [§]	1×10^4 to 6×10^5	≤ 13 ml	0.3 MPa, 3 bar, 42 psi	2.6 ml/min
Superdex 200 pg [§] (Bulk medium)	1×10^4 to 6×10^5	0.5% to 4% of total column volume	Column-dependent	10 to 50 cm/h

* HiLoad is packed with Superdex prep grade.

† For maximum resolution, apply as small sample volume as possible. Note that sample volumes less than 0.5% normally do not improve resolution.

‡ See Appendix 5 to convert linear flow (cm/h) to volumetric flow rates (ml/min) and vice versa.

§ prep grade.

** Typical pressure drop over the packed bed.



The maximum pressure drop over the packed bed is a typical value. Note that the actual value is individual for each column and needs to be determined (see *Setting column pressure limits*, Chapter 1).



Start with Superdex 200 Increase when the molecular weight of the protein of interest is unknown. Superdex 200 Increase or Superdex 200 prep grade are especially suitable for the separation of monoclonal antibodies from dimers and from contaminants of lower molecular weight, for example albumin and transferrin.



Start with Superdex Peptide or Superdex 30 prep grade for separations of peptides, oligonucleotides and small proteins below M_r 10 000.



Exposure to temperatures outside the range 4°C to 40°C will negatively affect the efficiency of the packed bed and the column will need to be repacked.

Separation examples

A critical step in MAb production and characterization is the analysis of aggregates and determination of purity of the monomeric fraction. Figure 2.10 illustrates the separation of a monoclonal mouse IgG from its aggregates using Superdex 200 Increase 10/300 GL. As shown, the aggregates and dimers were very well separated from the monomeric peak.

Column: Superdex 200 Increase 10/300 GL
Sample: Mouse IgG₁, 1.0 mg/ml
Sample volume: 15 μ l
Flow rate: 0.6 ml/min
Buffer: 100 mM sodium phosphate, 200 mM sodium chloride, pH 6.8
System: HPLC system

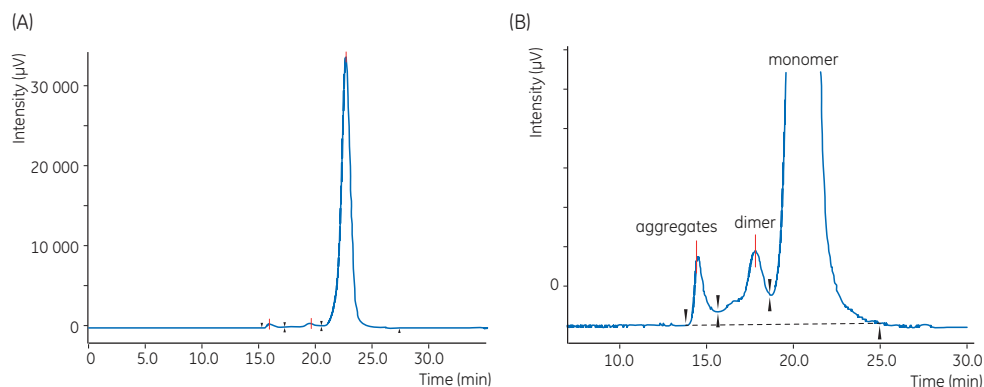


Fig 2.10. Analysis of monoclonal mouse IgG₁ antibody aggregates using Superdex 200 Increase 10/300 GL. (A) Chromatogram without magnification. (B) Magnified chromatogram showing details of aggregates, dimer, and monomer peaks.

For evaluation of detergents for further crystallization of a membrane protein, a rapid screening of maltoside detergents of variable acyl chain length—n-Dodecyl- β -maltoside (DDM), n-Undecyl- β -maltoside (UDM), n-Decyl- β -maltoside (DM), and n-Nonyl- β -maltoside (NM)—was performed on Superdex 200 Increase 5/150 GL. Purified recombinant membrane protein CE07 was run on Superdex 200 Increase 5/150 GL, equilibrated in respective detergent. The run time was approximately 6 min each. The results are shown in Figure 2.11. The DDM run was considered to give the most homogenous peak and is therefore a good choice for further crystallization experiments.

Column: Superdex 200 Increase 5/150 GL
 Sample: Recombinant integral membrane protein CE07
 Sample volume: 25 μ l
 Buffer: 20 mM HEPES, 150 mM sodium chloride, 5% glycerol,
 0.5 mM TCEP + maltoside detergent, pH 7.5
 Detergent: 0.03% DDM, 0.2% UDM, 0.01% DM, or 0.3% NM
 Flow rate: 0.5 ml/min
 System: ÄKTAmicro

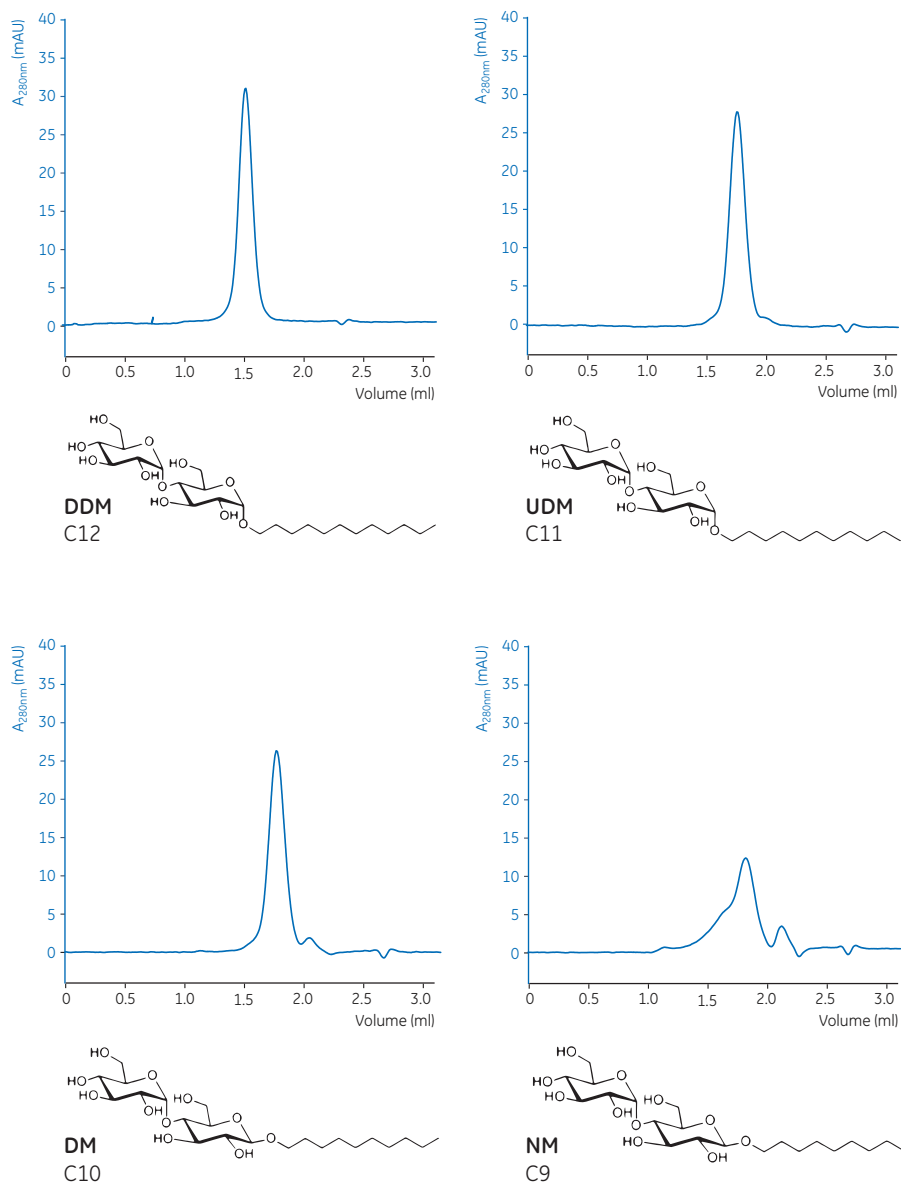


Fig 2.11. Rapid screening of detergents using Superdex 200 Increase 5/150 GL. Purified recombinant membrane protein CE07 was run in a column equilibrated with (A) DDM, (B) UDM, (C) DM, and (D) NM.

Superdex 75 5/150 GL was used to monitor complex formations. Trypsin and aprotinin were run separately as well as in a mixture on the column. Overlapping chromatograms of three runs are shown in Figure 2.12. The major peak eluting early in the mixture run corresponds to complex formation between trypsin and aprotinin.

Column: Superdex 75 5/150 GL
Sample: Trypsin (M_r 23 800), 11 mg/ml aprotinin (M_r 6 500), 3 mg/ml
Sample volume: 10 μ l
Buffer: PBS, pH 7.4
Flow rate: 0.3 ml/min

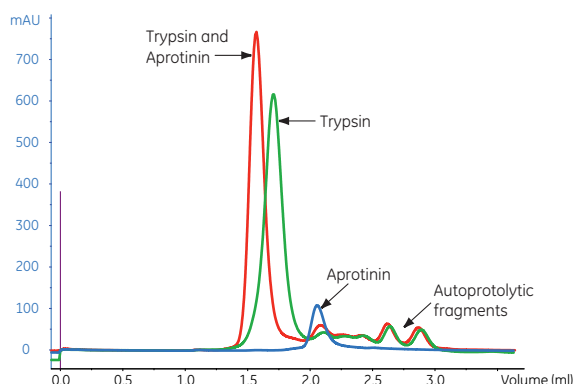


Fig 2.12. Monitoring of protein complex formation between trypsin and aprotinin.

Performing a separation

Buffer: 10 to 50 mM sodium phosphate, 150 mM sodium chloride, pH 7.0 to 7.4, or select the buffer in which the sample should be stored or solubilized for the next step.

Use 150 mM sodium chloride, or a buffer with equivalent ionic strength, to avoid pH-dependent ionic interactions with the matrix. At very low ionic strength, the presence of a small number of negatively charged groups on the medium can cause retardation of basic proteins.



The sample should be fully dissolved. Centrifuge or filter to remove particulate material (see Appendix 3). Always use degassed buffers and maintain a constant temperature during the run to avoid introducing air into the column.



Set an appropriate pressure limit on the chromatography system to avoid damage to the column packing.

First-time use or after long-term storage

1. Equilibrate the column with 2 column volumes of water to remove the storage solution. Use a low flow rate (Table 2.3) to avoid any gap formation.
2. For first-time use: Determine the column specific pressure limit according to section *Setting column pressure limits* (Chapter 1).
3. Perform a column efficiency test (see Appendix 1).
4. Equilibrate with 2 column volumes of buffer containing 150 mM sodium chloride at recommended flow rate during run (Table 2.2).
5. Apply a sample volume equivalent to 0.5% to 4% of the column volume. For most applications, the sample volume should not exceed 2% to achieve maximum resolution (up to 50 μ l for 3.2/300 GL and 5/150 GL, up to 500 μ l for 10/300 GL, up to 2.4 ml for HiLoad 16/600, and 6.4 ml for HiLoad 26/600). Note that small sample volume improves the resolution.

6. Elute with 1 column volume of buffer.
7. Before applying a new sample, re-equilibrate column with buffer until the baseline monitored at A_{280} is stable.

Column performance should be checked at regular intervals by determining the theoretical plate number per meter and peak symmetry.



See Appendix 1 for how to check column efficiency.



See Chapter 1 for advice on optimizing the separation.



Make sure to not exceed the pressure limits of the column and consider flow limitations (Table 1.3). This is particularly important when working at low temperatures, such as in a cold room, or when the column is used with 20% ethanol or other viscous solutions.



Exposure to temperatures outside the range 4°C to 40°C will negatively affect the efficiency of a packed bed and the column will need to be repacked.

Table 2.3. Recommended flow rates at different stages using prepacked columns containing Superdex Increase, Superdex, or HiLoad columns containing Superdex prep grade media

	Flow rates at room temperature				
	3.2/300 GL	5/150 GL	10/300 GL	HiLoad 16/600	HiLoad 26/600
First-time use or after long-term storage	0.05 ml/min	0.3 ml/min	0.5 ml/min	1 ml/min* (30 cm/h)	2.6 ml/min* (30 cm/h)
First-time use or after long-term storage (Superdex 200 Increase)	0.075 ml/min	0.3 ml/min	0.75 ml/min	N/A	N/A
Cleaning-in-place, CIP	0.02 ml/min	0.3 ml/min [†]	0.5 ml/min	0.8 ml/min (25 cm/h)	2.2 ml/min (25 cm/h)

* HiLoad: To save time, higher flow rate can be used for the equilibration with buffer: 1.6 ml/min and 4.3 ml/min for HiLoad 16/600 and HiLoad 26/600, respectively. Reduce the flow rate to the recommended flow rate during run before sample application.

[†] 0.13 ml/min for Superdex 200 Increase 5/150 GL.

Cleaning

1. Wash with 1 column volume of 0.5 M sodium hydroxide, alternatively 0.5 M acetic acid. Use a low flow rate during the entire CIP procedure (see Table 2.3).
2. Immediately wash with 1 column volume of distilled water followed by at least 2 column volumes of buffer until the baseline monitored at A_{280} and the pH of the eluent are stable.

Further equilibration might be necessary if the buffer contains detergent.



Routine cleaning after every 10 to 20 separations is recommended, but the frequency of cleaning will also depend on the nature of the samples being applied.

Removing severe contamination

1. Reverse the flow.
2. Wash with 4 column volumes of 1 M NaOH (to remove hydrophobic proteins or lipoproteins) followed by 4 column volumes of distilled water.

3. Wash with 0.5 column volume of 30% isopropanol to remove lipids and very hydrophobic proteins, followed by 2 column volumes of distilled water.
 4. Equilibrate the column with at least 5 column volumes of buffer, or until the baseline monitored at A_{280} and the pH of the eluent are stable, before beginning a new separation.
- For extreme cases of contamination, check the instructions supplied with the product.

Media characteristics

Matrix: Spherical composite of cross-linked agarose and dextran.

Table 2.4. Superdex media characteristics

Product	Efficiency*	pH stability [†]	Average particle size (µm)
Superdex 200 Increase [‡]	> 48 000	Long term: 3 to 12 Short term: 1 to 14	8.6
Superdex Peptide	≥ 30 000	Long term: 1 to 14 Short term: 1 to 14	13
Superdex 75 [‡]	≥ 30 000	Long term: 3 to 12 Short term: 1 to 14	13
Superdex 200 [‡]	≥ 30 000	Long term: 3 to 12 Short term: 1 to 14	13
Superdex 30 prep grade	≥ 13 000	Long term: 3 to 12 Short term: 1 to 14	34
Superdex 75 prep grade	≥ 13 000	Long term: 3 to 12 Short term: 1 to 14	34
Superdex 200 prep grade	≥ 13 000	Long term: 3 to 12 Short term: 1 to 14	34

* Theoretical plates m^{-1} (prepacked columns only).

[†] Long-term pH stability refers to the pH interval where the medium is stable over a long period of time without adverse side effects on its chromatography performance. Short-term pH stability refers to the pH interval for regeneration, cleaning-in-place and sanitization procedures. All ranges are GE Healthcare estimates.

[‡] Column length 300 mm.

Chemical stability

Superdex is stable in all commonly used aqueous buffers and additives such as detergents (1% SDS), and denaturing agents (8 M urea or 6 M guanidine hydrochloride).

The following solutions can be used for cleaning: up to 30% acetonitrile, up to 1 M sodium hydroxide, up to 70% ethanol (Superdex Increase, Superdex, Superdex 30 prep grade); up to 24% ethanol (Superdex 75 prep grade and Superdex 200 prep grade); up to 1 M acetic acid, 30% isopropanol or 0.1 M hydrochloric acid (Superdex Increase, Superdex, Superdex 30 prep grade).

Storage

Store unused media 4°C to 30°C in 20% ethanol (store Superdex 30 pg and Superdex 75 pg in 200 mM sodium acetate, 20% ethanol). Do not freeze.

For long-term storage, wash with 2 column volumes of distilled water followed by 2 column volumes of 20% ethanol (or 200 mM sodium acetate, 20% ethanol for Superdex 30 pg and Superdex 75 pg). Store at 4°C to 30°C.

Degas the ethanol/water mixture thoroughly and use a low flow rate. Connect the transport tool to the capillary tubing at the column outlet to prevent air from entering the column. Fill the transport tool up to approximately 50% of the transport tool volume.

Avoid changes in temperature, which can cause formation of air bubbles in the packing.

Chapter 3

Superose: broad fractionation range for laboratory scale

Superose are SEC media with high physical and chemical stability based on highly cross-linked porous agarose particles. Typical fractionation ranges for Superose are shown in Figure 3.1. Superose Increase is the next generation Superose medium and has improved performance even further by providing higher resolution at increased flow rates. This is achieved by using a high-flow agarose base matrix, which has higher flow/pressure tolerance, smaller bead size, and narrower particle size distribution.

The mechanical rigidity of Superose allows even viscous eluents, such as 8 M urea, to be run at relatively high flow rates. Under normal chromatography conditions, nonspecific interactions between proteins and Superose are negligible when using buffers with ionic strengths in the range 0.15 M to 1.5 M.

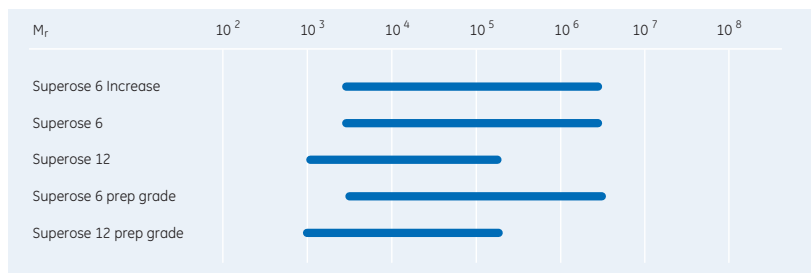


Fig 3.1. Fractionation ranges of Superose.

Some hydrophobic interactions have been noted, particularly for compounds such as smaller hydrophobic and/or aromatic peptides, membrane proteins and/or lipoproteins which can elute later than predicted. However, in some applications, these interactions can be an advantage for increasing the resolution of the separation.

Three types of Superose media are available: Superose Increase, Superose, and Superose prep grade.

Superose Increase

Superose 6 Increase has a small average particle size of 8.6 μm , which enables high-resolution fractionation in short run time, resulting in excellent analytical performance and high final purity. Superose 6 Increase has a broad fractionation range for molecular weights between 5000 and 5 000 000, and is especially valuable for its ability to separate large biomolecules, membrane proteins, and protein complexes. The selectivity curve for Superose 6 Increase is shown in Figure 3.2.

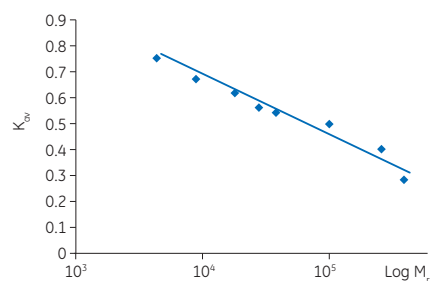


Fig 3.2. Superose 6 Increase selectivity curve for proteins.

Superose 6 Increase has higher resolution capabilities compared with the original Superose 6 medium. Figure 3.3 shows the result of the separation of standard proteins using Superose 6 Increase 10/300 GL and Superose 6 10/300 GL. The improved resolution observed with Superose 6 Increase can be attributed to the reduced bead size of Superose 6 Increase medium (8.6 μm) compared with the larger beads of Superose 6 (13 μm) as well as the narrower particle size distribution for Superose 6 Increase. The higher rigidity of the chromatography beads and thereby enhanced flow properties enable faster runs on Superose 6 Increase.

Columns: Superose 6 Increase 10/300 GL and Superose 6 10/300 GL
Sample: 1. Thyroglobulin (M_r 669 000), 3 mg/ml
2. Ferritin (M_r 440 000), 0.3 mg/ml
3. Aldolase (M_r 158 000), 3 mg/ml
4. Ovalbumin (M_r 44 000), 3 mg/ml
5. Ribonuclease A (M_r 13 700), 3 mg/ml
6. Aprotinin (M_r 6500), 1 mg/ml
Sample volume: 100 μl
Buffer: PBS (10 mM phosphate buffer, 140 mM sodium chloride, pH 7.4)
Flow rate: 0.5 ml/min
System: ÄKTAmicro

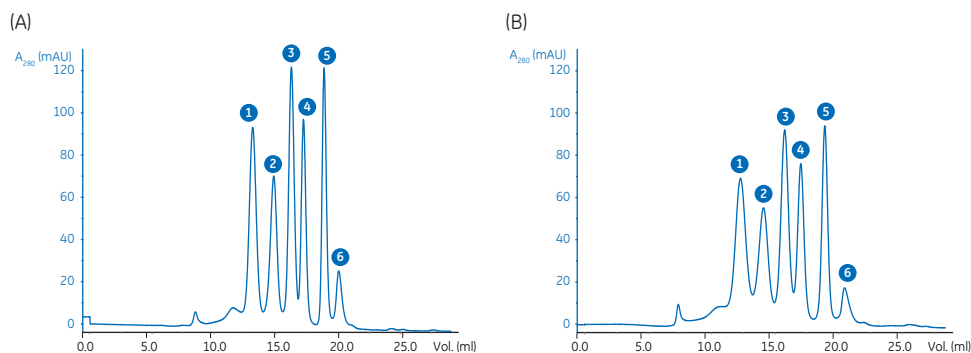


Fig 3.3. Chromatograms showing high-resolution SEC of six standard proteins on (A) Superose 6 Increase 10/300 GL and (B) Superose 6 10/300 GL.

The excellent reproducibility of Superose 6 Increase over the duration of 200 injections of IgG_{2b} and 200 cleaning-in-place (CIP) cycles can be seen in Figure 3.4.

Column: Superose 6 Increase 10/300 GL
Sample: 1. Thyroglobulin (M_r 669 000), 2 mg/ml
 2. Aldolase (M_r 158 000), 2 mg/ml
 3. Ovalbumin (M_r 44 000), 2 mg/ml
 4. Ribonuclease A (M_r 13 700), 0.6 mg/ml
Sample volume: 50 μ l
Buffer: PBS (10 mM phosphate buffer, 140 mM sodium chloride, pH 7.4)
Flow rate: 0.5 ml/min
System: ÄKTAexplorer 10

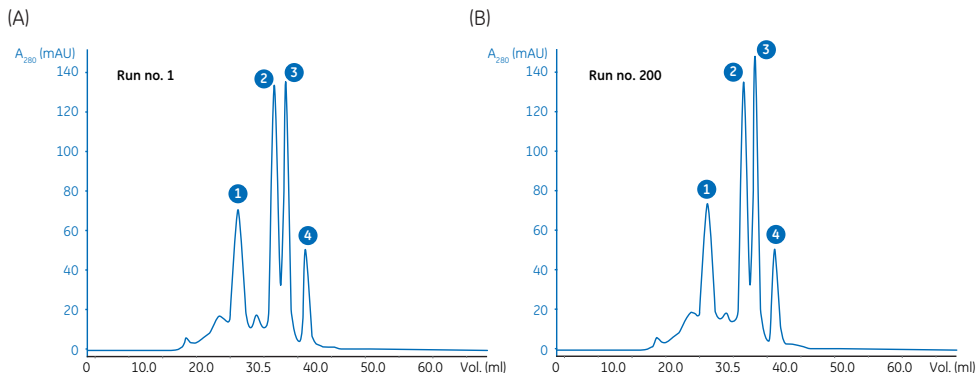


Fig 3.4. SEC of standard proteins on Superose 6 Increase 10/300 GL (A) before and (B) after 200 injections of IgG_{2b} including 20 CIP cycles with 0.5 M NaOH.

Superose 6 Increase media are prepacked in high-performance Tricorn glass columns as well as precision column format for small-scale preparative purification and analysis.

Superose

Superose 6 and Superose 12 have an average bead size of 13 and 11 μ m, respectively and have different selectivities (Fig 3.1). Superose 6 has a fractionation range for molecular weights between 5000 and 5 000 000. However, use of the next generation medium Superose 6 Increase (see earlier in this chapter) is recommended for this fractionation range since it offers increased resolution and shorter run times in comparison with Superose 6 (see comparison in Fig 3.3).

Superose 12 has a fractionation range for smaller molecular weights between 1000 and 300 000 (Fig 3.1).

Selectivity curves for Superose 6 and Superose 12 are shown in Figure 3.5.

Superose 6 and Superose 12 media are prepacked in high-performance Tricorn glass columns as well as precision column format for small-scale preparative purification and analysis (Table 3.1).

Superose prep grade

Superose prep 6 prep grade and Superose 12 prep grade have an average particle size of 30 μ m. The media have fractionation ranges of M_r 5000 to 5 000 000 and 1000 to 300 000, respectively. Superose prep grade media are designed for preparative applications in larger scales. The media are available in lab packs where the bead size of 30 μ m allows packing of larger columns at medium pressure and also gives increased tolerance to more crude samples, although filtration of the sample is still recommended. The selectivity curves for Superose and Superose prep grade media are shown in Figure 3.5.

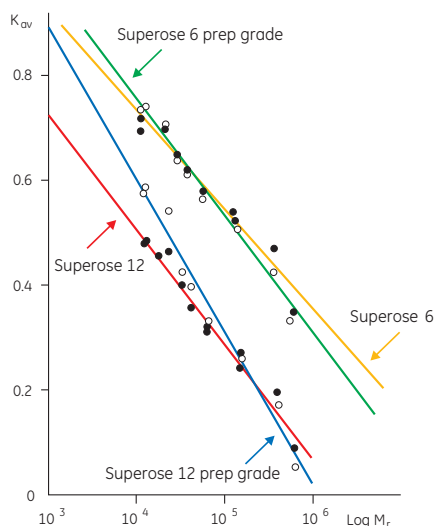


Fig 3.5. Superose 6 and 12 as well as Superose 6 and 12 prep grade selectivity curves for globular proteins.

Separation options

Superose is produced in different average particle sizes and with two different selectivities (Table 3.1). Superose 6 and 12, as well as Superose 6 Increase preppacked in 3.2/300 columns are an excellent choice when working with very small sample volumes and for high resolution small-scale separations. Superose 6 Increase 5/150 GL is the first choice for rapid screening and for applications where buffer consumption needs to be low. The column is also an excellent choice for purity checks. Superose 6 and 12 as well as Superose 6 Increase 10/300 GL are designed for high-resolution preparative-scale purification, protein analysis, and protein characterization.



Use the preppacked columns with Superose 6 Increase and Superose 12 for small-scale preparative purification and analytical runs.



Use bulk media of Superose 6 prep grade and Superose 12 prep grade for preparative purification.

Table 3.1. Separation options with Superose media

Product	Fractionation range, M_r (globular proteins)	Sample loading capacity*	Maximum pressure drop over the packed bed	Recommended operational flow rate [†]
Superose 6 Increase 10/300 GL	5×10^3 to 5×10^6	25 to 500 μ l	3.0 Mpa, 30 bar, 435 psi [‡]	0.5 ml/min
Superose 6 Increase 5/150 GL	5×10^3 to 5×10^6	4 to 50 μ	3.0 MPa, 30 bar, 435 psi [‡]	0.3 ml/min
Superose 6 Increase 3.2/300	5×10^3 to 5×10^6	4 to 50 μ l	3.0 Mpa, 30 bar, 435 psi [‡]	0.04 ml/min
Superose 6 10/300 GL	5×10^3 to 5×10^6	25 to 500 μ l	1.5 MPa, 15 bar, 217 psi	0.1 to 0.5 ml/min
Superose 6 3.2/300	5×10^3 to 5×10^6	< 50 μ l	1.2 MPa, 12 bar, 175 psi	0.04 ml/min
Superose 6 prep grade (Bulk medium)	5×10^3 to 5×10^6	0.5% to 4% of total column volume	Column-dependent	up to 40 cm/h
Superose 12 10/300 GL	1×10^3 to 3×10^6	25 to 500 μ l	3.0 MPa, 30 bar, 435 psi	0.5 ml/min
Superose 12 3.2/300	1×10^3 to 3×10^6	< 50 μ l	2.4 MPa, 24 bar, 350 psi	0.04 ml/min
Superose 12 prep grade (Bulk medium)	1×10^3 to 3×10^6	0.5% to 4% of total column volume	Column-dependent	up to 40 cm/h

* For maximum resolution, apply as a small sample volume as possible. Note that sample volumes less than 0.5% normally do not improve resolution.

[†] See Appendix 5 to convert linear flow (cm/h) to volumetric flow rates (ml/min) and vice versa.

[‡] Typical pressure drop over the packed bed.



The maximum pressure drop over the packed bed is a typical value. Note that the actual value is individual for each column and needs to be determined (see *Setting column pressure limits*, Chapter 1).

Separation examples

Figure 3.6 shows an example of the extremely small amounts of sample that can be analyzed on a Superose 12 3.2/300 column. A micropurification of 0.75 μl of human tears was performed using Superose 12 3.2/300.

Column: Superose 12 3.2/300
Sample: 0.75 μl of human tears
Buffer: 20 mM sodium phosphate, 500 mM sodium chloride, pH 5.3
Flow rate: 40 $\mu\text{l}/\text{min}$

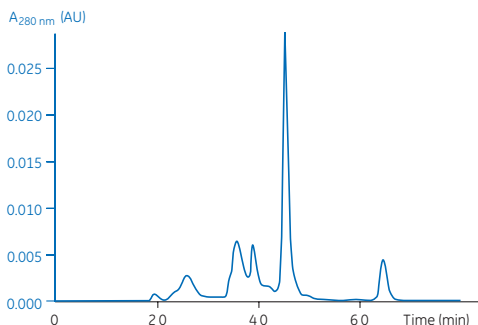


Fig 3.6. Microfractionation of 0.75 μl of human tears.

ATP synthetase complex from *E. coli* membrane was captured with Ni Sepharose 6 Fast Flow and further purified on Superose 6 Increase 5/150 GL. As seen in Figure 3.7, the resolution between aggregates (peak 1) and monomer ATP synthetase protein complex was good (peak 2), as well as separation from degradation products (peaks 3 and 4). In addition to small consumption of sample and buffer, the separation was achieved with low run time, yet sufficient resolution. The purified material was further used for structure and molecular mechanism studies.

Column: Superose 6 Increase 5/150 GL
Sample: ATP synthetase complex from *E. coli* membrane
Sample volume: 25 μl
Buffer: 20 mM Tris-HCl, 150 mM sodium chloride, 10% glycerol, 250 μM magnesium chloride, 0.05% dodecyl maltoside, pH 8.0
Flow rate: 0.15 ml/min
System: ÄKTAmicro in cold room

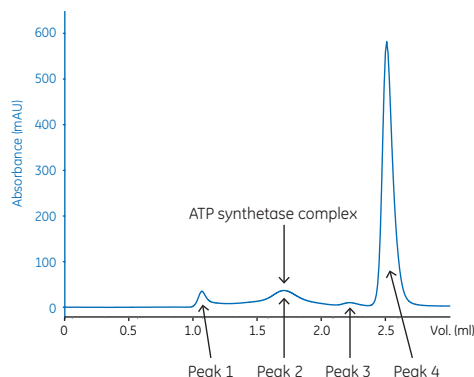




Fig 3.7. SEC using Superose 6 Increase 5/150 GL of ATP synthetase complex from *E. coli* membrane. Peak 1: Aggregates; Peak 2: Monomer ATP synthetase complex; Peak 3 and 4: Degradation products.

Performing a separation

Buffer: 10 to 50 mM sodium phosphate, 150 mM sodium chloride, pH 7.0 to 7.4, or select the buffer in which the sample should be stored or solubilized for the next step.

Use 150 mM sodium chloride or a buffer with equivalent ionic strength to avoid pH dependent nonionic interactions with the matrix. At very low ionic strength, the presence of a small number of negatively charged groups can cause retardation of basic proteins and exclusion of acidic proteins.

-  The sample should be fully dissolved. Centrifuge or filter to remove particulate material (see Appendix 3). Always use degassed buffers and maintain a constant temperature during the run to avoid introducing air into the column.
-  Set an appropriate pressure limit on the chromatography system to avoid damage to the column packing. Use lower flow rates for high viscosity solutions and low temperature (see Table 1.3).

First-time use or after long-term storage

1. Equilibrate the column with 2 column volumes of water at room temperature to remove the storage solution. Use a low flow rate (Table 3.2) to avoid any gap formation.
2. For first-time use: Determine the column specific pressure limit according to section *Setting column pressure limits* (Chapter 1).
3. Perform a column efficiency test (see Appendix 1).
4. Equilibrate with 2 column volumes of buffer at recommended flow rate during run (Table 3.1).
5. Apply a sample volume equivalent to between 0.5% and 4% of the column volume. For most applications the sample volume should not exceed 2% to achieve maximum resolution (up to 50 µl for 3.2/300 GL and 5/150 GL, up to 500 µl for 10/300 GL). Note that smaller sample volumes generally lead to improved resolution.
6. Elute with 1 column volume of buffer.



Before applying a new sample, re-equilibrate the column with buffer until the baseline monitored at A_{280} is stable.

Table 3.2. Recommended flow rates at different stages using prepacked columns containing Superose 6 Increase, Superose 6, and Superose 12 media

	Flow rates (ml/min) at room temperature		
	3.2/300 GL	5/150 GL	10/300 GL
First-time use or after long-term storage	0.04	0.25	0.5*
Cleaning-in-place, CIP	0.02	0.1	0.5

* Start with 0.2 ml/min for 0.5 column volumes.

Column performance should be checked at regular intervals by determining the theoretical plate number m^{-1} and peak a symmetry factor, A_s . See Appendix 1 for how to check column efficiency.

-  Ensure that the pressure limit of the column is not exceeded. This is particularly important when working at low temperatures, such as in a cold room, or when the column is used with 20% ethanol or other viscous solutions.
-  Exposure to temperatures outside the range 4°C to 40°C will negatively affect the efficiency of a packed bed and the column will need to be repacked.

Cleaning

1. Wash with 1 column volume of 0.5 M sodium hydroxide, alternatively 0.5 M acetic acid. Use a low flow rate during the entire CIP procedure. Use 0.2 M sodium hydroxide for Superose prep grade media.
2. Immediately wash with 1 column volume of distilled water followed by at least 2 column volumes of buffer until the baseline monitored at A_{280} and the pH of the eluent are stable.

For extreme cases of contamination, check the instructions supplied with the product.

In special cases, it might be necessary to change the bottom filter or to remove and discard the top 2 to 3 mm of the gel. These operations must be done with extreme care to avoid serious loss of resolution. Note that Precision Columns (3.2/300) should not be opened.

Superose prep grade may be autoclaved repeatedly at 121°C, pH 7 for 30 min without significantly affecting its chromatographic properties. The medium must be removed from the column as autoclaving can damage column components. Note that Precision Columns (3.2/300) cannot be repacked.

Media characteristics

Matrix: Cross-linked agarose.

Table 3.2 Superose media characteristics

Product	Efficiency (theoretical plates m^{-1})*	pH stability†	Average particle size (μm)
Superose 6 Increase‡	> 48 000	Long term: 3 to 12 Short term: 1 to 14	8.6
Superose 6	\geq 30 000	Long term: 3 to 12 Short term: 1 to 14	13
Superose 6 prep grade	§	Long term: 3 to 12 Short term: 1 to 14	30
Superose 12	\geq 40 000	Long term: 3 to 12 Short term: 1 to 14	11
Superose 12 prep grade	§	Long term: 3 to 12 Short term: 1 to 14	30

* *Prepacked columns only.*

† *Long-term pH stability refers to the pH interval where the medium is stable over a long period of time without adverse side effects on its chromatography performance. Short-term pH stability refers to the pH interval for regeneration, cleaning-in-place, and sanitization procedures. All ranges are GE Healthcare estimates.*

‡ *Column length 300 mm.*

§ *A minimum column efficiency of 10 000 m^{-1} should be expected for a well-packed column.*

Chemical stability

Superose is stable in all commonly used aqueous buffers and additives such as detergents, denaturing agents (8 M urea or 6 M guanidine hydrochloride), and 30% acetonitrile.

Storage

Store unused media 4°C to 30°C in 20% ethanol. Do not freeze.

For long-term storage, wash with 2 column volumes of distilled water followed by 2 column volumes of 20% ethanol at low flow rate. Store at 4°C to 30°C.

Degas the ethanol/water mixture thoroughly and use a low flow rate. Connect the transport tool to the capillary tubing at the column outlet to prevent air from entering the column. Fill the tool up to approximately 50% of the total volume.

Avoid changes in temperature, which can cause air bubbles in the packing.

Chapter 4

Sephacryl: fast, high-recovery separations at laboratory and industrial scale

Sephacryl High Resolution (HR) media provide a useful alternative to Superdex prep grade for applications that require a slightly broader fractionation range, as shown in Figure 4.1. High chemical stability and tolerance of high flow rates make Sephacryl well suited for industrial use.

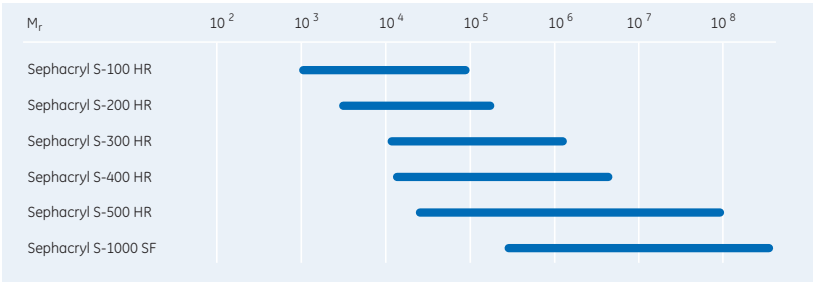


Fig 4.1. Fractionation ranges for Sephacryl HR.

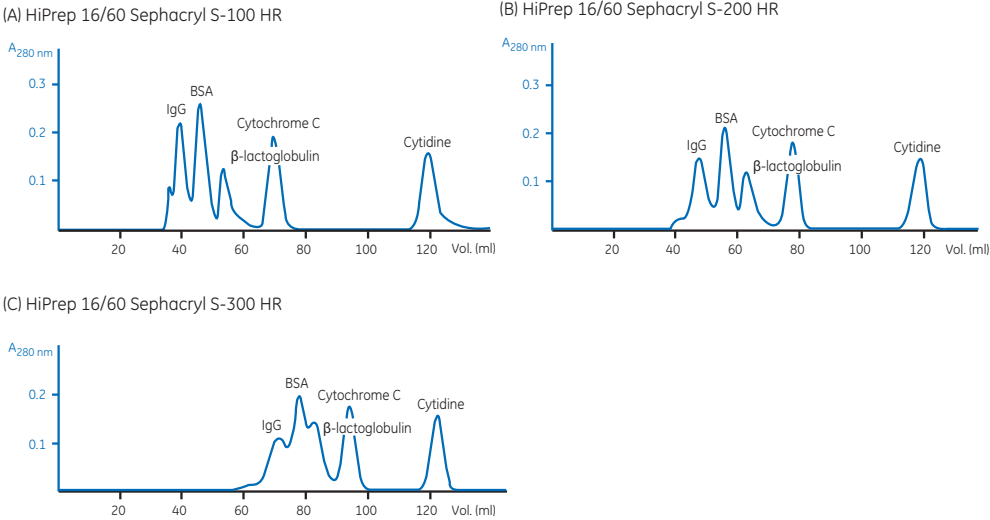


Fig 4.2. Sephacryl is available as bulk media and in prepacked columns.

Figure 4.3 shows comparisons of the different selectivities of Sephacryl HR.

Typical selectivity and pressure-flow relationship curves for Sephacryl are shown in Figures 4.4 and 4.5.

Column: (A) HiPrep 16/60 Sephacryl S-100 HR
 (B) HiPrep 16/60 Sephacryl S-200 HR
 (C) HiPrep 16/60 Sephacryl S-300 HR
Sample: 500 µl of a mixture comprising IgG (M_r 160 000), BSA (M_r 67 000),
 β-lactoglobulin (M_r 35 000), cytochrome C (M_r 12 400), and cytidine (M_r 240)
Buffer: 50 mM sodium phosphate, 150 mM sodium chloride, pH 7.0
Flow rate: 0.8 ml/min (24 cm/h)



Column: (D) HiPrep 16/60 Sephacryl S-400 HR
 (E) HiPrep 16/60 Sephacryl S-500 HR
Sample: (D) 1.2 ml of a sample containing three dextrans; $M_r > 20 \times 10^6$,
 M_r 270 000, and M_r 12 000
 (E) 1.2 ml of a sample containing three dextrans, $M_r > 20 \times 10^6$,
 M_r 1.8×10^6 , and M_r 25 000
Buffer: 250 mM sodium chloride
Flow rate: 0.5 ml/min (15 cm/h)

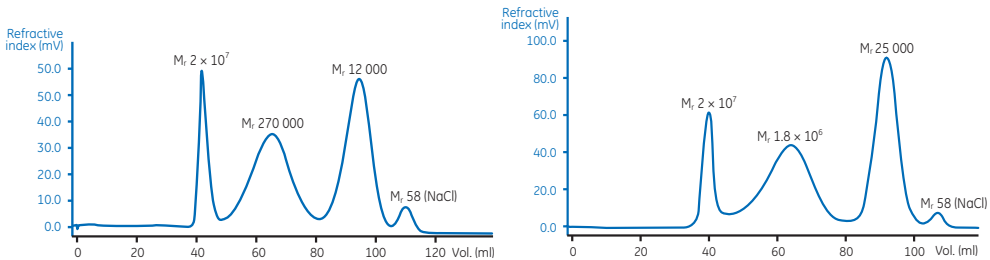


Fig 4.3. Comparison of the selectivity of the five different prepacked HiPrep Sephacryl HR columns.

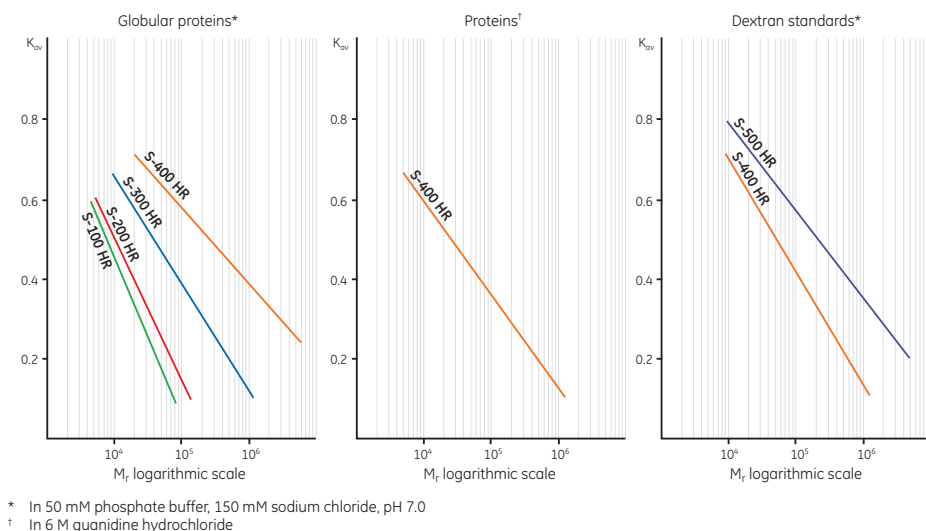


Fig 4.4. Selectivity curves for Sephacryl HR chromatography media.

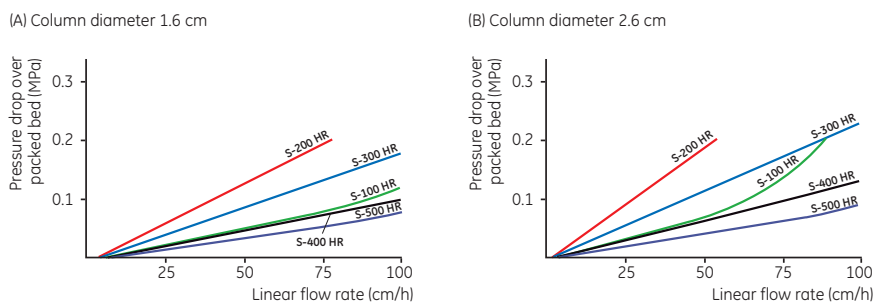


Fig 4.5. Pressure drop as a function of flow rate for Sephacryl HR. Bed height approximately 60 cm, distilled water, temperature 25°C. To calculate the volumetric flow rate, multiply the linear flow by the cross-sectional area of the column (2 cm² for XK 16 or 5.3 cm² for XK 26).

Sephacryl HR is a composite medium prepared by covalently cross-linking allyl dextran with N,N'-methylene bisacrylamide to form a hydrophilic matrix of high mechanical strength. The porosity of the medium, determined by the dextran component, has been controlled to yield five different selectivities. The mechanical rigidity of Sephacryl HR allows even relatively viscous eluents, such as 8 M urea, to be run at practical flow rates. Under normal chromatography conditions (A_{280} , 50 mM phosphate, 150 mM sodium chloride, pH 7.0) Sephacryl S-100 HR gave yields of at least 96% of the following substances: Blue Dextran 2000, ferritin, catalase, aldolase, BSA, ovalbumin, β -lactoglobulin A+B, chymotrypsinogen A, myoglobin, lysozyme, ribonuclease A, and cytochrome C. An ionic strength of at least 150 mM is recommended for optimal results.

Separation options

Five Sephacryl HR chromatography media are available as prepacked columns and in bulk packs (Table 4.1).

Table 4.1. Separation options with Sephacryl media

Product	Fractionation range, M_r (globular proteins)	Fractionation range, M_r (dextrans)	Sample loading capacity*	Maximum pressure drop over the packed bed	Recommended operation flow [†]
HiPrep 16/60 Sephacryl S-100 HR	1×10^3 to 1×10^5		≤ 5 ml	0.15 MPa, 1.5 bar, 21 psi	0.5 ml/min
HiPrep 26/60 Sephacryl S-100 HR	1×10^3 to 1×10^5		≤ 13 ml	0.15 MPa, 1.5 bar, 21 psi	1.3 ml/min
Sephacryl S-100 HR (Bulk medium)	1×10^3 to 1×10^5		0.5% to 4% of total column volume	Column-dependent	10 to 35 cm/h
HiPrep 16/60 Sephacryl S-200 HR	5×10^3 to 2.5×10^5	1×10^3 to 8×10^4	≤ 5 ml	0.15 MPa, 1.5 bar, 21 psi	0.5 ml/min
HiPrep 26/60 Sephacryl S-200 HR	5×10^3 to 2.5×10^5	1×10^3 to 8×10^4	≤ 13 ml	0.15 MPa, 1.5 bar, 21 psi	1.3 ml/min
Sephacryl S-200 HR (Bulk medium)	5×10^3 to 2.5×10^5	1×10^3 to 8×10^4	0.5% to 4% of total column volume	Column-dependent	10 to 35 cm/h
HiPrep 16/60 Sephacryl S-300 HR	1×10^4 to 1.5×10^6	2×10^3 to 4×10^5	≤ 5 ml	0.15 MPa, 1.5 bar, 21 psi	0.5 ml/min
HiPrep 26/60 Sephacryl S-300 HR	1×10^4 to 1.5×10^6	2×10^3 to 4×10^5	≤ 13 ml	0.15 MPa, 1.5 bar, 21 psi	1.3 ml/min
Sephacryl S-300 HR (Bulk medium)	1×10^4 to 1.5×10^6	2×10^3 to 4×10^5	0.5% to 4% of total column volume	Column-dependent	10 to 35 cm/h
HiPrep 16/60 Sephacryl S-400 HR	2×10^4 to 8×10^6	1×10^4 to 2×10^6	≤ 5 ml	0.15 MPa, 1.5 bar, 21 psi	0.5 ml/min
HiPrep 26/60 Sephacryl S-400 HR	2×10^4 to 8×10^6	1×10^4 to 2×10^6	≤ 13 ml	0.15 MPa, 1.5 bar, 21 psi	1.3 ml/min
Sephacryl S-400 HR (Bulk medium)	2×10^4 to 8×10^6	1×10^4 to 2×10^6	0.5% to 4% of total column volume	Column-dependent	10 to 35 cm/h
HiPrep 16/60 Sephacryl S-500 HR		4×10^4 to 2×10^7	≤ 5 ml	0.15 MPa, 1.5 bar, 21 psi	0.5 ml/min
HiPrep 26/60 Sephacryl S-500 HR		4×10^4 to 2×10^7	≤ 13 ml	0.15 MPa, 1.5 bar, 21 psi	1.3 ml/min
Sephacryl S-500 HR (Bulk medium)		4×10^4 to 2×10^7	0.5% to 4% of total column volume	Column-dependent	10 to 35 cm/h
Sephacryl S-1000 SF (Superfine, bulk medium)			0.5% to 4% of total column volume	not determined	2 to 30 cm/h

* For maximum resolution, apply as small sample volume as possible. Note that sample volumes less than 0.5% normally do not improve resolution.

[†] See Appendix 5 to convert linear flow (cm/h) to volumetric flow rates (ml/min) and vice versa.

Separation examples

Figures 4.6 and 4.7 are examples of separations performed on Sephacryl media.

Column: HiPrep 26/60 Sephacryl S-100 HR
Sample: 1 ml of a mixture containing bovine insulin chain A (M_r 2532) and chain B (M_r 3496), 0.5 mg/ml of each
Buffer: 50 mM sodium phosphate, 150 mM sodium chloride, pH 7.0
Flow rate: 2.0 ml/min (22 cm/h)

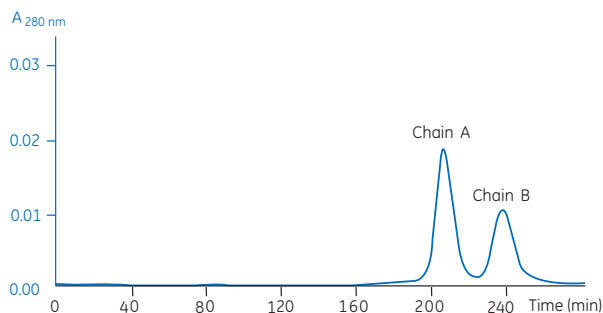


Fig 4.6. Separation of insulin chains on HiPrep 26/60 Sephacryl S-100 HR.

Column: BP 113/120 containing Sephacryl S-200 HR, bed height 100 cm
Sample: IgG fraction from previous ion-exchange step (sample volume equivalent to 1% of V_t , (V_t = column volume))
Buffer: 50 mM Tris-HCl, 150 mM sodium chloride, pH 7.5
Flow rate: 7.5 cm/h

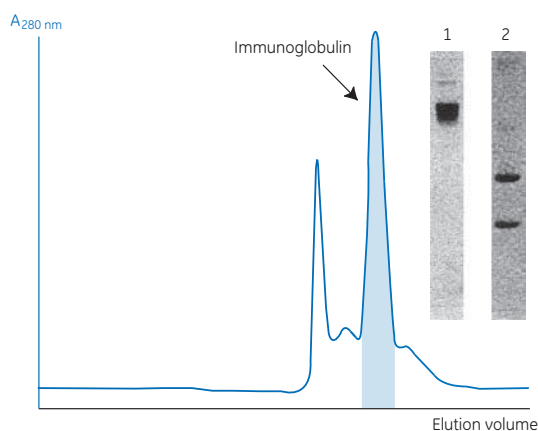


Fig 4.7. Purification of monoclonal antibodies on Sephacryl S-200 HR. Inset shows analysis by gradient the immunoglobulin pool. Lane 1, native sample; lane 2, sample reduced with 2-mercaptoethanol.

Performing a separation

Buffer: 50 mM sodium phosphate, 150 mM sodium chloride, pH 7.2 or select the buffer in which the sample should be stored or solubilized for the next step.

Use 150 mM sodium chloride, or a buffer with equivalent ionic strength, to avoid pH dependent nonionic interactions with the matrix. At very low ionic strength, the presence of a small number of negatively charged groups can cause retardation of basic proteins and exclusion of acidic proteins.



The sample should be fully dissolved. Centrifuge or filter to remove particulate material (Appendix 3). Always use degassed buffers and maintain a constant temperature during the run to avoid introducing air into the column.



Set an appropriate pressure limit on the chromatography system to avoid damage to the column packing. Use lower flow rates for high viscosity solutions and low temperature (see Table 1.3).

First-time use or after long-term storage

1. Equilibrate the column with at least 0.5 column volumes of distilled water at 15 cm/h (0.5 ml/min for 16/60 column or 1.3 ml/min for 26/60).
2. Equilibrate with 2 column volumes of buffer at 30 cm/h (1.0 ml/min for 16/60 column or 2.6 ml/min for 26/60).
3. Reduce flow to 15 cm/h and, for optimal resolution, apply a sample volume equivalent to 1% of the column volume (1.2 ml for 16/60 column or 3.2 ml for 26/60). Sample volumes between 0.5% and 4% can be applied.
4. Elute with 1 column volume of buffer.
5. Before applying a new sample-re-equilibrate column with 1 column volume of buffer at 30 cm/h until the baseline monitored at A_{280} is stable.



Column performance should be checked at regular intervals by determining the theoretical plate number per meter and peak symmetry. Prepacked columns are supplied with recommended values. See Appendix 1 on how to check column efficiency.

See Chapter 1 for advice on optimizing the separation.



Exposure to temperatures outside the range 4°C to 40°C will negatively affect the efficiency of a packed bed and the column will need to be repacked.

Cleaning

1. Wash with 0.5 column volumes of 0.2 M sodium hydroxide at a flow of 15 cm/h (0.5 ml/min for column 16/60 or 1.3 ml/min for 26/60) to remove most nonspecifically adsorbed proteins.
2. Re-equilibrate immediately with 2 column volumes of buffer or until the baseline monitored at A_{280} and the pH of the eluent are stable.

Further equilibration might be necessary if the buffer contains detergent.



Routine cleaning after every 10 to 20 separations is recommended, but the frequency of cleaning will also depend on the nature of the samples being applied.

If required, Sephacryl HR may be autoclaved repeatedly at 121°C, pH 7, for 30 min without significantly affecting its chromatographic properties. The medium must be removed from the column as autoclaving can damage column components. Note that HiPrep columns cannot be repacked.

To remove severe contamination

Reverse the flow and wash at a flow rate of 10 cm/h (0.3 ml/min for column 16/60 or 0.8 ml/min for 26/60) at room temperature using the following solutions:

1. Wash with 0.25 column volumes of 0.5 M sodium hydroxide (to remove hydrophobic proteins or lipoproteins) followed by 4 column volumes of distilled water.
2. Wash with 0.5 column volumes of 30% isopropanol (to remove lipids and very hydrophobic proteins), followed by 2 column volumes of distilled water.

For extreme cases of contamination, check the instructions supplied with the product.



Reversing flow through a column packed with Sephacryl media should only be considered under cases of severe contamination. Reversing the flow can cause channeling through the packed bed leading to poor resolution, reduced efficiency, and the need to repack the column. Professionally packed columns are less likely to be affected, but extreme care must be taken.

Media characteristics

Matrix: Cross-linked copolymer of allyl dextran and N,N'-methylene bisacrylamide.

Table 4.2 Sephacryl media characteristics

Product	Efficiency: theoretical plates m ⁻¹ (prepacked columns only)	pH stability*	Average particle size (µm)
Sephacryl S-100 HR	≥ 5000	Long term: 3 to 11 Short term: 2 to 13	47
Sephacryl S-200 HR	≥ 5000	Long term: 3 to 11 Short term: 2 to 13	47
Sephacryl S-300 HR	≥ 5000	Long term: 3 to 11 Short term: 2 to 13	47
Sephacryl S-400 HR	9000	Long term: 3 to 11 Short term: 2 to 13	47
Sephacryl S-500 HR	9000	Long term: 3 to 11 Short term: 2 to 13	47
Sephacryl S-1000 SF (Superfine)	†	Long term: 3 to 11 Short term: 2 to 13	65

* Long-term pH stability refers to the pH interval where the medium is stable over a long period of time without adverse side effects on its chromatographic performance. Short-term pH stability refers to the pH interval for regeneration, cleaning-in-place, and sanitization procedures. All ranges are GE Healthcare estimates.

† Not determined.

Chemical stability

Sephacryl HR is stable in all commonly used aqueous buffers and additives such as detergents (1% SDS) and denaturing agents (8 M urea or 6 M guanidine hydrochloride). The medium is also stable in 30% acetonitrile, 0.5 M sodium hydroxide, up to 24% ethanol, up to 1 M acetic acid, and up to 30% isopropanol.

Storage

Store unused media 4°C to 30°C in 20% ethanol. Do not freeze.

Columns can be left connected to a chromatography system with a low flow rate (0.01 ml/min) of buffer passing through the column to prevent bacterial growth or the introduction of air into the column which would negatively affect the packing.

For long-term storage, wash with 4 column volumes of distilled water followed by 4 column volumes of 20% ethanol. Store at 4°C to 30°C.

Degas the ethanol/water mixture thoroughly and use a low flow rate, checking the back pressure as the column equilibrates.

Avoid changes in temperature which can cause air bubbles in the packing.

Chapter 5

Sephadex: desalting, buffer exchange, and sample clean up

SEC based on Sephadex enables group separation of biomolecules that are above the exclusion limit of the medium, from contaminants such as salts, dyes, and radioactive labels. Sephadex is prepared by cross-linking dextran with epichlorohydrin.

The different types of Sephadex vary in their degree of cross-linking and hence in their degree of swelling and selectivity for specific molecular sizes (Table 5.4).

Sephadex G-10 is well-suited for the separation of biomolecules such as peptides ($M_r > 700$) from smaller molecules ($M_r < 100$).

Sephadex G-25 is recommended for the majority of group separations involving globular proteins. These media are excellent for removing salt and other small contaminants away from molecules that are greater than M_r 5000. Using different particle sizes enables columns to be packed according to application requirements (Table 5.1). The particle size determines the flow rates and the maximum sample volumes that can be applied. For example, smaller particles give higher column efficiency (narrow, symmetrical peaks), but might need to be run more slowly as they create higher operating pressures.

Sephadex G-50 is suitable for the separation of molecules from $M_r > 30\,000$ to molecules of $M_r < 1\,500$ such as labeled protein or DNA from unconjugated dyes. The medium is often used to remove small nucleotides from longer chain nucleic acids.

Table 5.1. Typical applications areas for Sephadex G-25 media

Sephadex G-25	Application
Superfine	For highest column efficiency (highest resolution), but operating pressures increase
Fine	For laboratory-scale separations
Coarse and Medium	Use when a high flow rate at a low operating pressure is essential, e.g., in large-scale applications
Coarse	For batch procedures



Fig 5.1. Prepacked Sephadex G-25 columns: left HiPrep 26/10 Desalting, right HiTrap Desalting 5 ml.



Use desalting/buffer exchange when needed, before purification, between purification steps, and/or after purification. These methods are faster than dialysis. However, each extra step can reduce yield and desalting often dilutes the sample (centrifugation protocols do not dilute samples).



Use Sephadex G-25 products to remove salts and other low molecular weight compounds from proteins with $M_r > 5000$ and Sephadex G-10 products for proteins with $M_r > 700$.

Desalting provides several advantages over dialysis. Dialysis is generally a slow technique that requires large volumes of buffer and carries the risk that material and target protein activity will be lost during handling. When desalting, sample volumes of up to 30% of the total volume of the desalting column can be processed. The high speed and capacity of the separation allows even relatively large sample volumes to be processed rapidly and efficiently in the laboratory, as illustrated in Figure 5.2. Sample concentration does not influence the separation as long as the concentration of proteins does not exceed approximately 70 mg/ml when using normal aqueous buffers, and provided that the target protein is stable and soluble at the concentration used. Use 100 mM ammonium acetate or 100 mM ammonium hydrogen carbonate if volatile buffers are required.



When desalting is the first chromatography step, the sample should first be clarified; centrifugation and/or filtration is recommended.

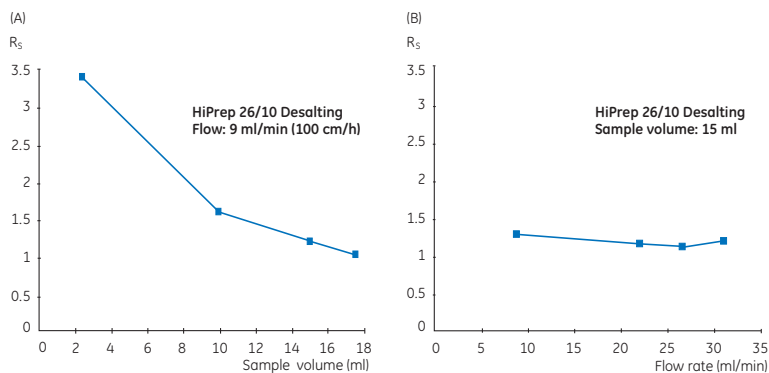


Fig 5.2. (A) Influence of sample volume on resolution. (B) Influence of flow rate on resolution.

Desalting columns are used not only to remove low molecular weight contaminants such as salt, but also for buffer exchange before and after different chromatography techniques and for the rapid removal of reagents to terminate a reaction. Examples of group separations include:

- Removal of phenol red from culture fluids prior to anion exchange chromatography or nucleic acid preparations
- Removal of unincorporated nucleotides during DNA sequencing
- Removal of free low-molecular weight labels
- Termination of reactions between macromolecules and low molecular weight reactants
- Removal of products, cofactors, or inhibitors from enzymes
- Removal of unreacted radiolabels such as [α - 32 P] adenosine triphosphate (ATP) from nucleic acid labeling reactions

Separation options

For group separations the medium should be selected so that the high molecular weight molecules are eluted at the void volume with minimum peak broadening or dilution and minimum time on the column. The lowest molecular weight substances should appear by the time one column volume of buffer has passed through the column.

Sephadex media are available in prepacked columns (also spin columns), microplates, and in bulk media packs (Table 5.2).

Table 5.2. Group separation options with Sephadex media

	Columns and 96-well plates	Chromatography medium	Loaded volume (ml)	Eluted volume (ml)	Dilution factor	Operation
	PD SpinTrap™ G-25	Sephadex G-25 Medium	0.07 to 0.13	0.07 to 0.13*	No dilution	Centrifuge
	PD MultiTrap™ G-25	Sephadex G-25 Medium	0.07 to 0.13	0.07 to 0.13*	No dilution	Centrifuge
	PD MiniTrap™ G-25	Sephadex G-25 Medium	0.2 to 0.5	0.1 to 0.5	No dilution	Centrifuge
			0.1 to 0.5	1.0	2 to 10	Gravity flow
	PD MidiTrap™ G-25	Sephadex G-25 Medium	0.75 to 1.0	0.5 to 1.0	No dilution	Centrifuge
			0.5 to 1.0	1.5	1.5 to 3	Gravity flow
	PD-10 Desalting columns	Sephadex G-25 Medium	1.75 to 2.5	1.0 to 2.5	No dilution	Centrifuge
			1.0 to 2.5	3.5	1.5 to 3.5	Gravity flow
	PD MiniTrap G-10	Sephadex G-10 Medium	0.1 to 0.3	0.5	1.7 to 5	Gravity flow
	PD MidiTrap G-10	Sephadex G-10 Medium	0.4 to 1.0	1.2	1.2 to 3.0	Gravity flow
	HiTrap Desalting	Sephadex G-25 Superfine	0.25	1.0	4 (approx.)	Syringe/pump/system
			0.5	1.5	3 (approx.)	Syringe/pump/system
			1.0	2.0	2 (approx.)	Syringe/pump/system
			1.5 (max.)	2.0	1.3 (approx.)	Syringe/pump/system
	2× HiTrap Desalting	Sephadex G-25 Superfine	3.0 (max.)	4.0 to 5.0	1.3 to 1.7	Syringe/pump/system
	3× HiTrap Desalting	Sephadex G-25 Superfine	4.5 (max.)	6.0 to 7.0	1.3 to 1.7	Syringe/pump/system
	HiPrep 26/10 Desalting	Sephadex G-25 Fine	10	10 to 15	1.0 to 1.5	Pump/system
			15 (max.)	15 to 20	1.0 to 1.3	Pump/system
	2× HiPrep 26/10 Desalting	Sephadex G-25 Fine	30 (max.)	30 to 40	1.0 to 1.3	Pump/system
	3× HiPrep 26/10 Desalting	Sephadex G-25 Fine	45 (max.)	45 to 55	1.0 to 1.2	Pump/system
	4× HiPrep 26/10 Desalting	Sephadex G-25 Fine	60 (max.)	60 to 70	1.0 to 1.2	Pump/system

- Contains Sephadex G-25 Medium
- Contains Sephadex G-10 Medium
- Contains Sephadex G-25 Superfine
- Contains Sephadex G-25 Fine

* Applied volume = eluted volume; For sample volumes less than 100 µl it is recommended to apply a stacker volume of 30 µl equilibration buffer after the sample has fully absorbed.

For convenience and reliable performance, use prepacked Sephadex columns such as HiTrap Desalting 5 ml and HiPrep 26/10 Desalting.



Always use disposable columns if there is a risk of biological or radioactive contamination or when any possibility of carryover between samples is unacceptable.

The type of equipment available and the sample volume to be processed also govern the choice of prepacked column, as shown in Figure 5.3.


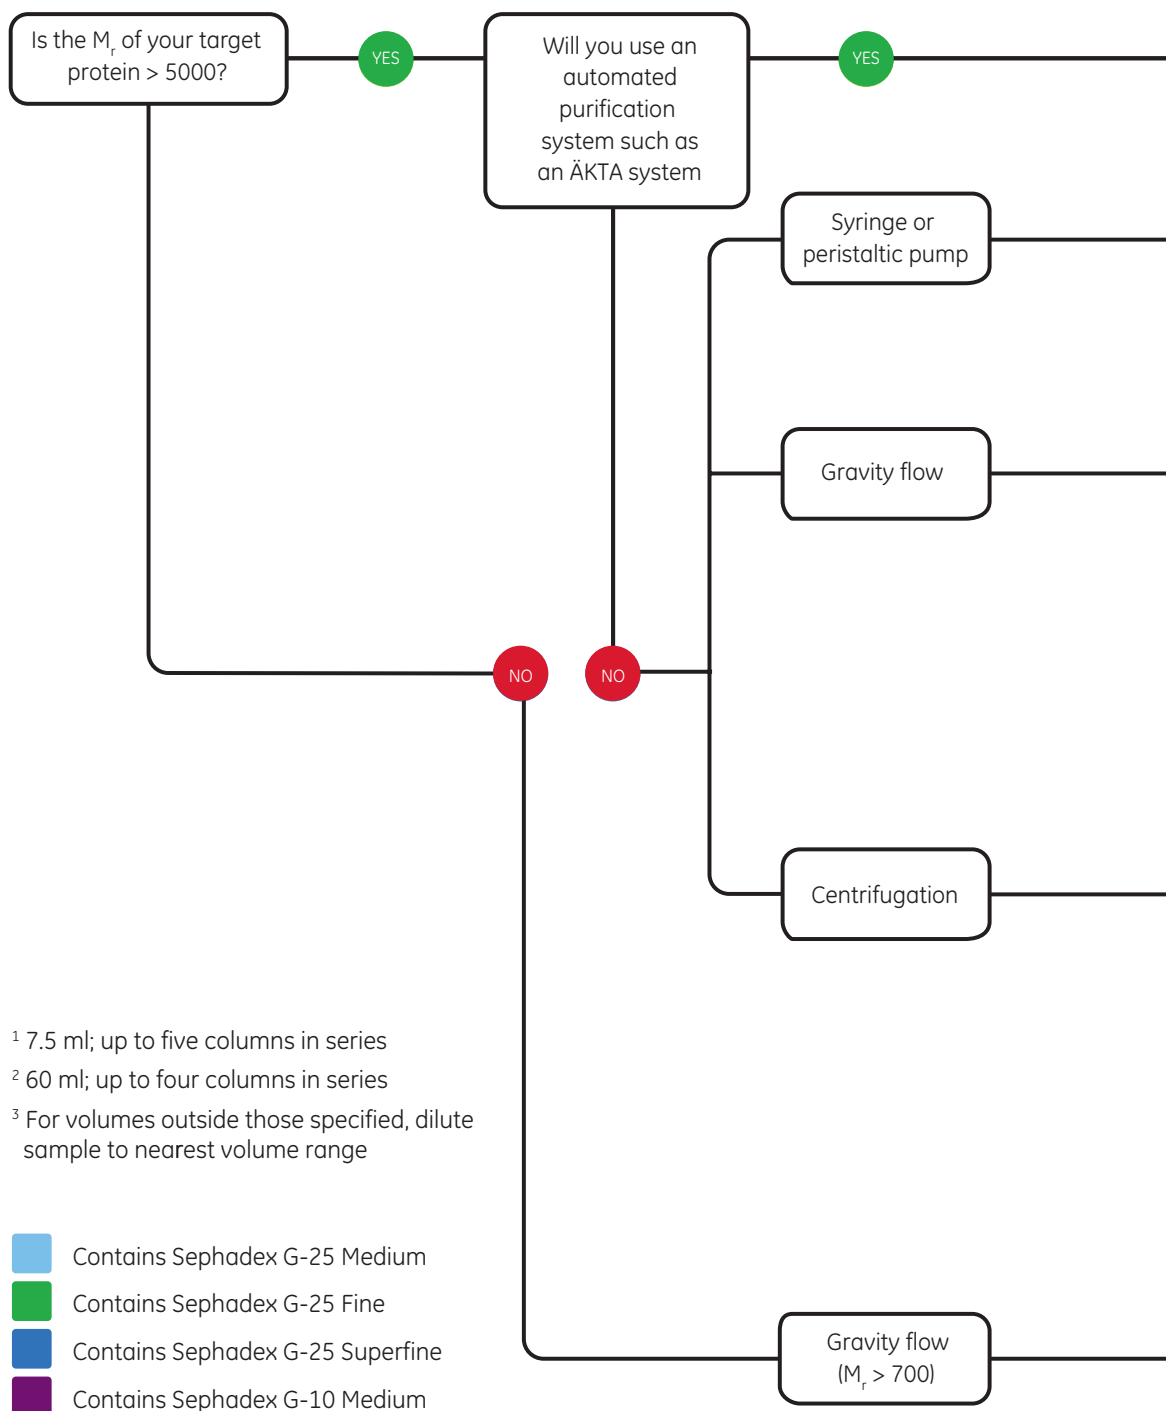


Fig 5.3. Selecting prepac columns for desalting and buffer exchange.

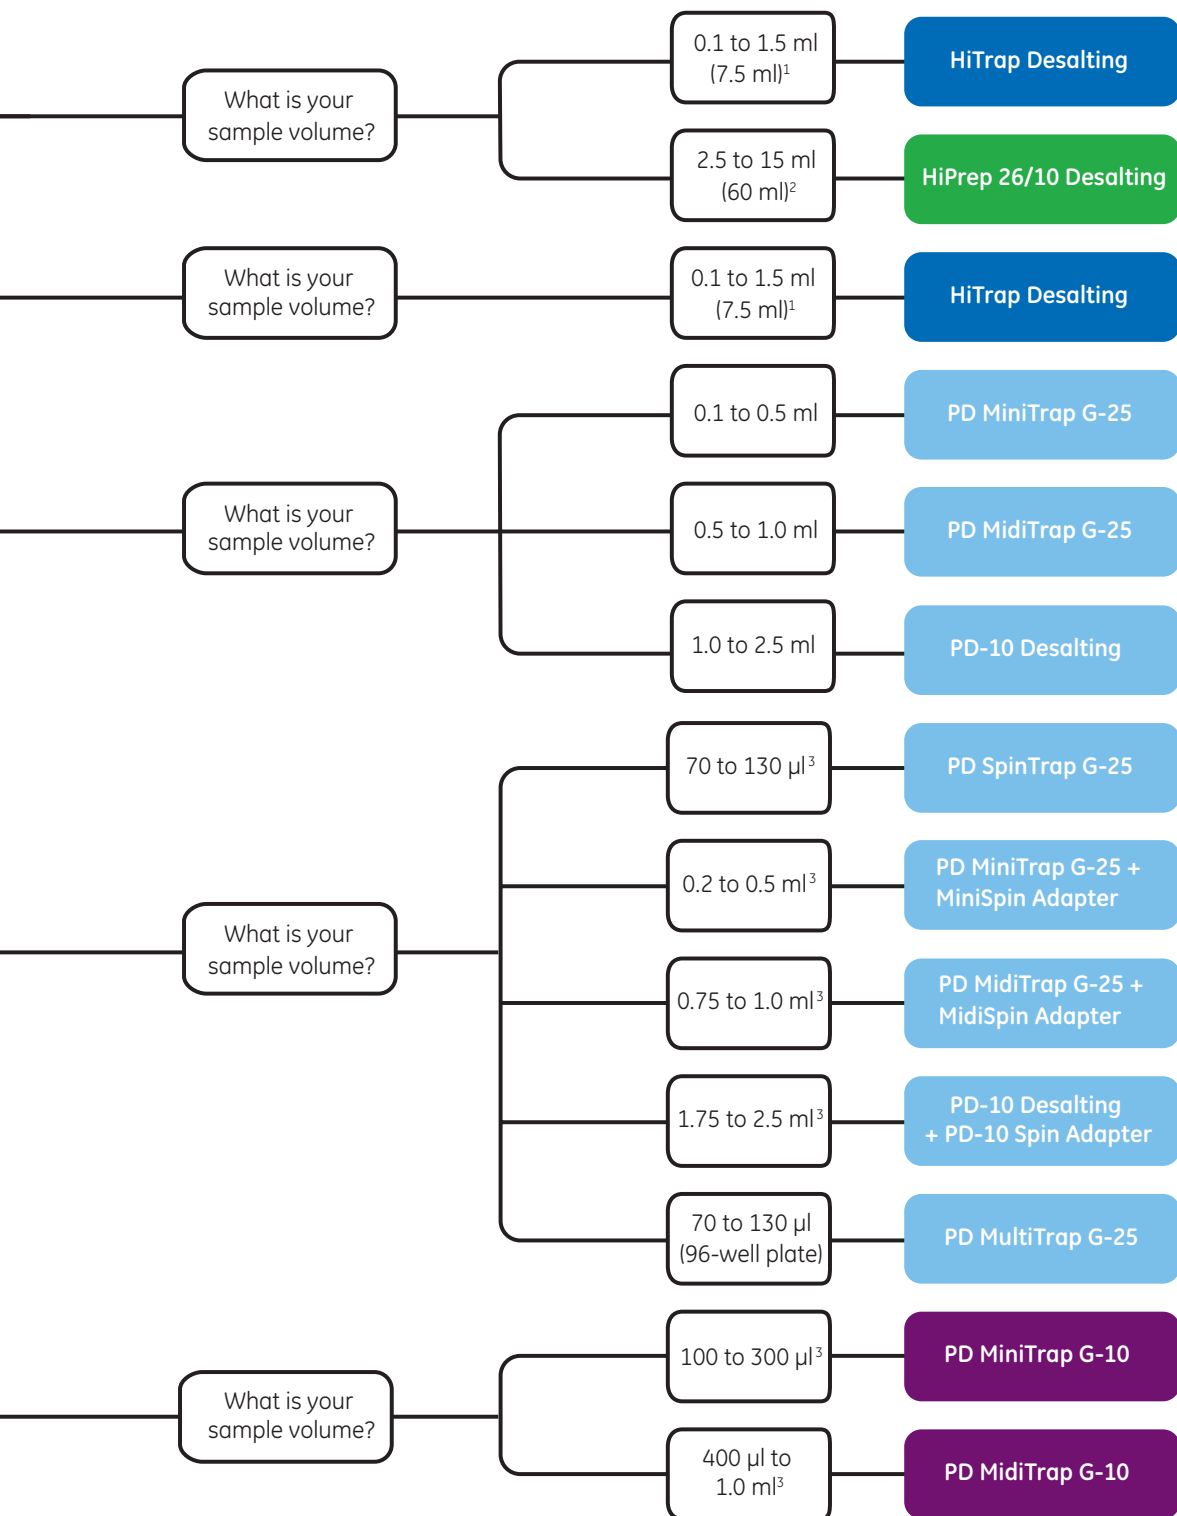

Separation examples

Figures 5.4 and 5.5 show examples of separations performed on Sephadex media.

Sample: (Histidine)₆-tagged protein eluted from HiTrap Chelating HP with 20 mM sodium phosphate, 500 mM sodium chloride, 500 mM imidazole, pH 7.4
Column: HiTrap Desalting 5 ml
Buffer: 20 mM sodium phosphate, 150 mM sodium chloride, pH 7.0

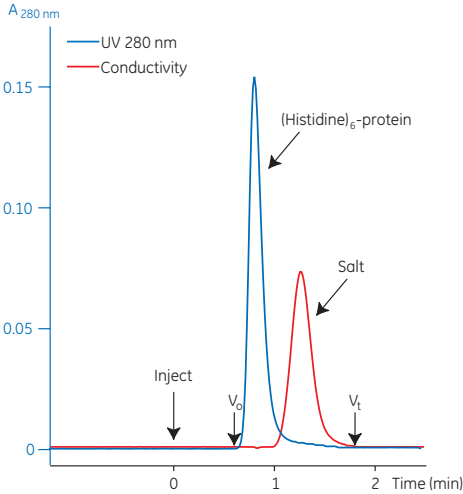


Fig 5.4. Desalting a (Histidine)₆ fusion protein using HiTrap Desalting 5 ml on ÄKTApriime. The UV (protein) and conductivity (salt) traces enable pooling of the desalted fractions and facilitate optimization of the separation.

Column: HiPrep 26/10 Desalting
Sample: 2 mg/ml BSA, 0.07 mg/ml N-Hydroxysuccinimide (NHS) in 50 mM sodium phosphate, 150 mM sodium chloride, pH 7.0. Filtered through a 0.45 µm filter
Sample volume: 13 ml
Buffer: 50 mM sodium phosphate, 150 mM sodium chloride, pH 7.0
Flow rate: 31 ml/min (350 cm/h)

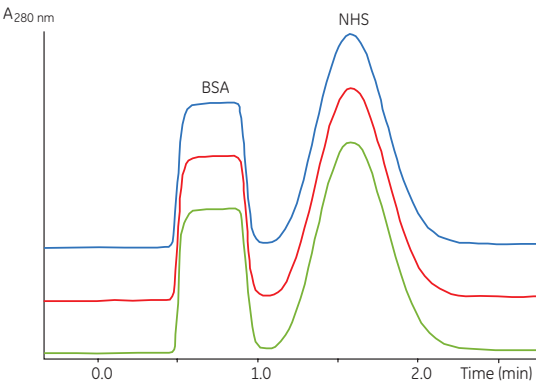


Fig 5.5. Reproducible removal of N-hydroxysuccinimide from BSA.

Performing a separation

Desalting and buffer exchange can take less than 5 min/sample with greater than 95% recovery for most proteins.



To prevent possible ionic interactions the presence of a low salt concentration (25 mM sodium chloride) is recommended during desalting and in the final sample buffer. Volatile buffers such as 100 mM ammonium acetate or 100 mM ammonium hydrogen carbonate can be used if it is necessary to avoid the presence of sodium chloride.



The sample should be fully dissolved. Centrifuge or filter to remove particulate material (Appendix 3). Always use degassed buffers to avoid introducing air into the column.



Sample concentration up to 70 mg/ml protein should not influence the separation when using normal aqueous buffers.

If possible, use a chromatography system with both a UV and a conductivity monitor to facilitate optimization of the sample loading. The elution of the protein peak at A_{280} and the appearance of the salt peak can be followed exactly and different separations can be easily compared, as shown in Figure 5.6.

If conductivity cannot be monitored and recovery of completely desalted sample is the major requirement, apply sample volumes of between 15% and 20% of the total column volume.

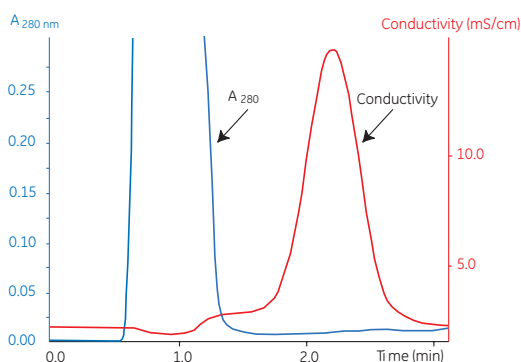


Fig 5.6. Buffer exchange of mouse plasma on HiPrep 26/10 Desalting.

General considerations

Small-scale desalting of samples

For sample volumes ranging from 0.2 to 2.5 ml, it is possible to run multiple samples in parallel with PD-10 Desalting, PD MidiTrap G-25, and PD MiniTrap G-25 columns. Two different protocols are available for these columns: one for manual use on the laboratory bench and one for use together with a standard centrifuge in combination with a Spin Adapter. For smaller proteins ($M_r > 700$), PD MiniTrap G-10 and PD MidiTrap G-10 columns may be used.

For smaller sample volumes in the range of 70 to 130 μ l, multiple samples can be run on PD SpinTrap G-25 spin columns together with a microcentrifuge or PD MultiTrap G-25 96-well plate using centrifugation for extraction. Although possible to perform, using PD MultiTrap G-25 with vacuum is not recommended due to reduced reproducibility compared with operation using centrifugation.

Desalting larger sample volumes using HiTrap and HiPrep columns

Connect up to three HiTrap Desalting columns in series to increase the sample volume capacity. For example, two columns allow a sample volume of 3 ml, and three columns allow a sample volume of 4.5 ml (Table 5.2).

Connect up to four HiPrep 26/10 Desalting columns in series to increase the sample volume capacity. For example, two columns allow a sample volume of 30 ml, and four columns allow a sample volume of 60 ml. Even with four columns in series, the sample can be processed in 20 to 30 min without back pressure problems.

Buffer preparation

For substances carrying charged groups, an eluent containing a buffer salt is recommended. A salt concentration of at least 150 mM is recommended to prevent possible ionic interactions with the chromatography medium. Sodium chloride is often used for this purpose. Often a buffer with 25 to 50 mM concentration of the buffering substance is sufficient. At salt concentrations above 1 M, hydrophobic substances can be retarded or can bind to the chromatography medium.

At even higher salt concentrations, > 1.5 M ammonium sulfate, the column packing shrinks.

Sample preparation

Sample concentration does not influence the separation as long as the viscosity does not differ by more than a factor of 1.5 from that of the buffer used. This corresponds to a maximum concentration of 70 mg/ml for proteins, when normal, aqueous buffers are used. The sample should be fully solubilized. Centrifuge or filter (0.45 µm filter) immediately before loading to remove particulate material if necessary.

Buffer exchange

Protein solubility often depends on pH and/or ionic strength (salt concentration), and the exchange of buffer can therefore result in precipitation of the protein. Also, protein activity can be lost if the change of pH takes it outside of the range where the protein is active. Samples that have been obtained after purification will usually be free from particles, unless the purified protein or a contaminant has been aggregated.

The protocols in the following sections describe desalting and buffer exchange using different formats of prepacked columns.

HiTrap Desalting columns



Fig 5.7. HiTrap Desalting column allows easy and efficient group separations with a syringe, pump, or chromatography system.

HiTrap Desalting is a 5 ml column (Fig 5.7) packed with the SEC medium Sephadex G-25 Superfine, which is based on cross-linked dextran beads. The fractionation range for globular proteins is between M_r 1000 and 5000, with an exclusion limit of approximately M_r 5000. This ensures group separations of proteins/peptides larger than M_r 5000 from molecules with a molecular weight less than M_r 1000.

HiTrap Desalting can be used with aqueous solutions in the pH range 2 to 13. The prepacked medium is stable in all commonly used buffers, solutions of urea (8 M), guanidine hydrochloride (6 M), and all nonionic and ionic detergents. Lower alcohols (methanol, ethanol, propanol) can be used in the buffer or the sample, but we recommend that the concentration be kept below 25% v/v. Prolonged exposure (hours) to pH below 2 or above 13, or to oxidizing agents, should be avoided.

The recommended range of sample volumes is 0.1 to 1.5 ml when complete removal of low molecular weight components is desired. The separation is not affected by the flow rate, in the range of 1 to 10 ml/min. The maximum recommended flow rate is 15 ml/min. Separations are easily performed with a syringe, pump, or chromatography system. Up to three columns can be connected in series, allowing larger sample volumes to be handled. To avoid cross-contamination, use the column only with the same type of sample.

Manual purification with a syringe



Fig 5.8. Using HiTrap columns with a syringe. (A) Prepare buffers and sample. Remove the column's top cap and twist off the end. (B) Equilibrate the column, load the sample, and begin collecting fractions. (C) Wash and elute, continuing to collect fractions.

1. Fill the syringe with binding buffer. Remove the stopper and connect the column to the syringe (use the connector supplied) "drop to drop" to avoid introducing air into the column.
2. Remove the snap-off end at the column outlet.
3. Equilibrate the column with 5 column volumes of binding buffer.
4. Apply the pretreated sample using a syringe fitted to the Luer connector on the column. For optimal results, use a flow rate of 0.2 to 1 ml/min (1 ml column) and 0.5 to 5 ml/min (5 ml column) during sample application*.
5. Wash with 5 to 10 column volumes of binding buffer or until no material appears in the effluent. Maintain a flow rate of 1 to 2 ml/min (1 ml column) and 5 to 10 ml/min (5 ml column) for washing. Optional: collect the flowthrough (in 1 ml fractions for the 1 ml column and 2 ml fractions for the 5 ml column) and reserve until the procedure has been successfully completed. Retain a sample for analysis by SDS-PAGE to measure the efficiency of protein binding to the medium.
6. Elute with 5 to 10 column volumes of elution buffer. Maintain a flow rate of 0.2 to 1 ml/min (1 ml column) and 0.5 to 5 ml/min (5 ml column) for elution.
7. After elution, regenerate the column by washing it with 3 to 5 column volumes of binding buffer. The column is now ready for a new purification.

* 1 ml/min corresponds to approximately 30 drops/min when using a syringe with a HiTrap 1 ml column; 5 ml/min corresponds to approximately 120 drops/min when using a HiTrap 5 ml column



For large sample volumes, a peristaltic pump can be used to apply sample and buffers.

Simple desalting with ÄKTAprime plus

ÄKTAprime plus contains preprogrammed templates for individual HiTrap Desalting 5 ml and HiPrep 26/10 Desalting columns.



Fig 5.9. ÄKTAprime plus.



Prepare at least 500 ml of each buffer.

1. Follow the instructions supplied on the ÄKTAprime plus cue card to connect the column and load the system with binding buffer.
2. Select the Application Template.
3. Start the method.
4. Enter the sample volume and press OK to start.

(A)



(B)



(C)



(D)



Fig 5.10. Typical procedures using ÄKTAprime plus. (A) Prepare the buffers. (B) Connect the column. (C) Prepare the fraction collector. (D) Load the sample.

Desalting on a gravity-feed PD-10 column

Buffer preparation

1. Remove top cap and pour off the excess liquid.
2. Cut off the bottom tip.
3. Place column in the Desalting Workmate supplied onto the plastic tray and equilibrate with 25 ml buffer. Discard the eluent.
4. Add a total sample volume of 2.5 ml. If the sample volume is less than 2.5 ml, add buffer to reach a final volume of 2.5 ml. Discard the eluent.
5. Add 3.5 ml buffer to elute high molecular weight components and collect the eluent.



Using the standard procedure described above protein yield is typically greater than 95% with less than 4% salt (low molecular weight) contamination. The dilution factor is 1:4.



Sephadex G-10 can be packed into empty PD-10 columns and run in the same manner as PD-10 Desalting columns.

Optimization of desalting

1. When possible, select a prepacked column that is suited to the volume of sample that needs to be desalted (see Separation Options). For the majority of separations, the instructions supplied ensure satisfactory results and very little optimization should be necessary.
2. Ensure that buffer conditions are optimal for the separation.
3. Select the highest flow rate recommended. Figure 5.11 shows an example of the influence of flow rate on group separation.
4. Determine the maximum sample volume that can be loaded. Figure 5.12 shows an example of the influence of sample volume on group separation.

Column: HiTrap Desalting 5 ml
Sample: Bovine serum albumin, 2 mg/ml in 500 mM NaCl, 50 mM sodium phosphate, pH 7.0
Sample volume: 0.8 ml
Buffer: 50 mM sodium phosphate, 150 mM sodium chloride, pH 7.0
Flow rate: 1.7, 3.3, 6.7, 10.0, 13.3, 16.7, 20.0 ml/min

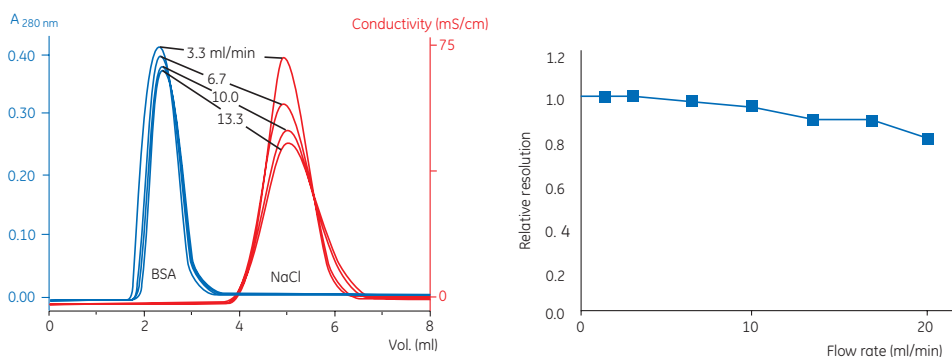


Fig 5.11. Influence of flow rate on separation using a HiTrap Desalting column.

Column: HiTrap Desalting 5 ml
Sample: BSA, 2 mg/ml in 50 mM sodium phosphate, 500 mM sodium chloride, pH 7.0
Buffer: 50 mM sodium phosphate, 150 mM sodium chloride, pH 7.0
Sample volume: 0.8, 1.3, 1.7, 2.2 ml
Flow rate: 5 ml/min

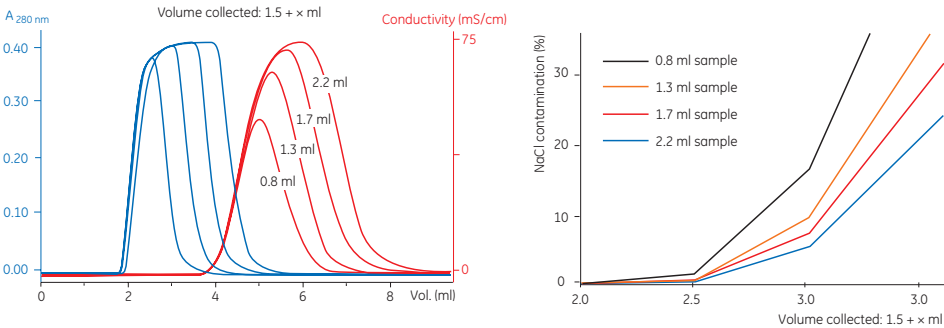


Fig 5.12. Influence of sample volume on separation using a HiTrap Desalting column.

As the sample volume increases (up to a maximum of 30% of the total column volume) the dilution factor decreases and there might be a slight increase in the amount of salt remaining in the sample after elution.



Sample volumes up to 30% of the total column volume give a separation with minimal sample dilution. Larger sample volumes can be applied, but resolution will be reduced.

Scale-up and processing larger sample volumes

Connecting columns in series increases the effective column volume and so increases sample loading capacity. Table 5.3 shows the sample loading capacities and dilution factors when using prepacked desalting columns alone or in series, see also Figure 5.13 for HiTrap application examples.

Table 5.3. Selection guide for desalting/buffer exchange columns

Column	Loaded volume (ml)	Eluted volume (ml)	Dilution factor	Operation
HiPrep 26/10 Desalting	10	10 to 15	1 to 1.3	pump
	15 (max.)	15 to 20	1 to 1.5	pump
2 × HiPrep 26/10 Desalting	30 (max.)	30 to 40	1 to 1.3	pump
3 × HiPrep 26/10 Desalting	45 (max.)	40 to 55	1 to 1.2	pump
4 × HiPrep 26/10 Desalting	60 (max.)	60 to 70	1 to 1.2	pump
HiTrap Desalting	0.25	1.0	4	syringe/pump
	0.5	1.5	3	syringe/pump
	1.0	2.0	2	syringe/pump
	1.5 (max.)	2.0	1.3	syringe/pump
2 × HiTrap Desalting	3.0	4 to 5	1.3 to 1.7	syringe/pump
3 × HiTrap Desalting	4.5 (max.)	6 to 7	1.3 to 1.7	syringe/pump
PD-10 Desalting columns	1.5	3.5	2.3	gravity
	2.0	3.5	1.7	gravity
	2.5	3.5	1.4	gravity

Increasing sample loading capacity from 1.5 ml up to 7.5 ml

Column: HiTrap Desalting, 1 × 5 ml, 3 × 5 ml, 5 × 5 ml
Sample: 2 mg/ml of BSA in 50 mM sodium phosphate, 500 mM sodium chloride, pH 7.0
Sample volume: 28% × V_t (1.4, 4.3, and 7.1 ml, respectively)
Buffer: 50 mM sodium phosphate, 150 mM sodium chloride, pH 7.0
Flow rate: 5 ml/min

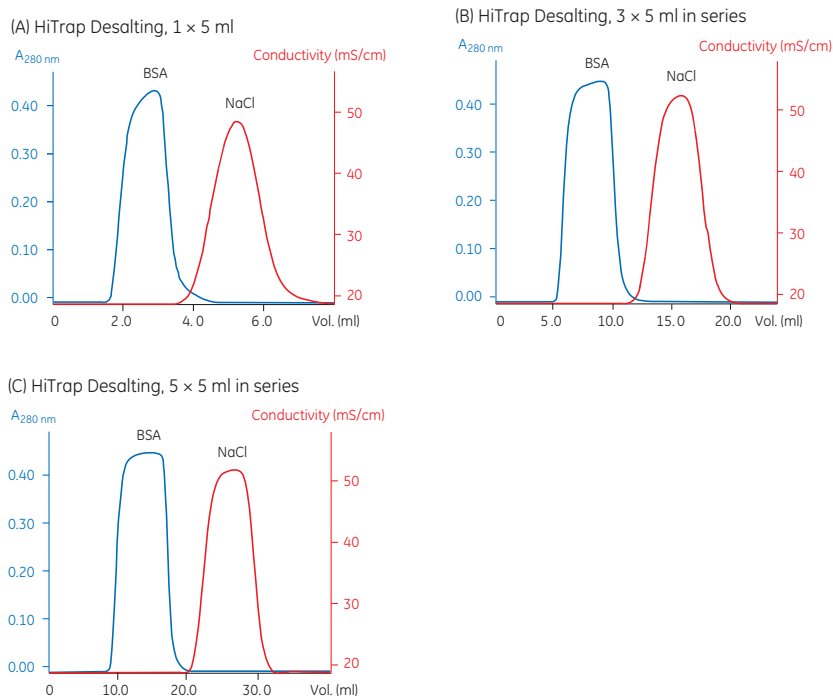


Fig 5.13. Scale-up using HiTrap columns connected in series.

Increasing sample loading capacity from 15 ml up to 60 ml

Connect HiPrep 26/10 Desalting columns in series. With two columns, a sample volume of 30 ml can be applied, and four columns allow a sample volume of 60 ml (Fig 5.14). Even with four columns in series, high flow rates can be maintained without causing back pressure difficulties so that up to 60 ml of sample can be processed in 20 to 30 min.



Fig 5.14. Four HiPrep 26/10 Desalting columns connected in series.

For sample volumes greater than 60 ml

Select a suitable particle size of Sephadex G-25, rehydrate and pack into a short, wide column to facilitate high flow rates and rapid recovery of desalted materials. See Appendix 1 for details on column packing. The particle size determines the flow rates and sample volumes that can be applied, as shown in Figure 5.15.

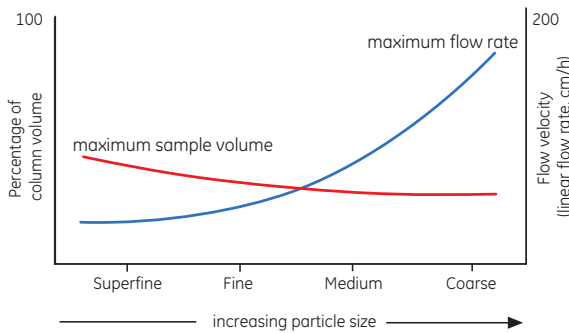


Fig 5.15 Sephadex G-25: recommended sample volumes and flow rates vary with particle size.

- Use Superfine grade with a bed height of approximately 15 cm when requiring the highest efficiencies.
- Use Fine grade with an approximate bed height of 15 cm for laboratory-scale separations.
- Use Medium and Coarse grades for preparative processes where a high flow rate at a low operating pressure is essential. Pack in a column less than 50 cm in bed height. The Coarse grade is suitable for batch procedures.

Media characteristics

Sephadex is prepared by cross-linking dextran with epichlorohydrin. Variations in the degree of cross-linking create the different Sephadex media and influence their degree of swelling and their selectivity for specific molecular sizes.

Table 5.4. Sephadex media characteristics

Product	Fractionation range, M_r (globular proteins)	pH stability*	Bed volume ml/g dry Sephadex	Maximum operating flow	Particle size in 150 mM sodium chloride (μm)
Sephadex G-10 Medium	$< 7 \times 10^2$	Long term: 2 to 13 Short term: 2 to 13	2 to 3	Darcy's law†	55 to 165
Sephadex G-25 Superfine	1×10^3 to 5×10^3	Long term: 2 to 13 Short term: 2 to 13	4 to 6	Darcy's law†	15 to 88
Sephadex G-25 Fine	1×10^3 to 5×10^3	Long term: 2 to 13 Short term: 2 to 13	4 to 6	Darcy's law†	17 to 132
Sephadex G-25 Medium	1×10^3 to 5×10^3	Long term: 2 to 13 Short term: 2 to 13	4 to 6	Darcy's law†	80 to 260
Sephadex G-25 Coarse	1×10^3 to 5×10^3	Long term: 2 to 13 Short term: 2 to 13	4 to 6	Darcy's law†	87 to 510
Sephadex G-50 Fine	1×10^3 to 3×10^4	Long term: 2 to 10 Short term: 2 to 13	9 to 11	Darcy's law†	34 to 208

* Long-term pH stability refers to the pH interval where the medium is stable over a long period of time without adverse side effects on its chromatography performance. Short-term pH stability refers to the pH interval for regeneration, cleaning-in-place, and sanitization procedures. All ranges are GE Healthcare estimates.

† In practice this means that the pressure/flow considerations that must be made when using other SEC media do not apply to Sephadex. Doubling flow rate will double column pressure. See Appendix 2 for an explanation of Darcy's law.

Column packing

See Appendix 1.

Cleaning

PD-10, SpinTrap, MultiTrap, MiniTrap, MidiTrap, and HiTrap Desalting columns are disposable, but, depending on the type of sample and if cross-contamination is not a concern, they can be re-used a few times.

For HiPrep 26/10 Desalting columns proceed as follows:

1. Wash the column with 2 column volumes of 0.2 M sodium hydroxide or a solution of a nonionic detergent (typically 0.1% to 0.5% Triton X-100 dissolved in distilled water or 0.1 M acetic acid) at a flow rate of 10 ml/min. Ensure that the pressure drop does not exceed 0.15 MPa (1.5 bar, 22 psi).
2. Wash the column with 5 column volumes of distilled water at a flow rate of 15 ml/min.
3. Before use, re-equilibrate the column with at least 5 column volumes of buffer until the UV baseline and pH are stable.

To remove precipitated proteins and peptides, fill the column with 1 mg pepsin/ml in 0.1 M acetic acid, 0.5 M sodium chloride and leave at room temperature overnight or 1 h at 37°C. Repeat the normal cleaning procedure above.

Chemical stability

Sephadex is stable in all commonly used aqueous buffers and additives such as ionic and nonionic detergents, as well as denaturing agents (8 M urea or 6 M guanidine hydrochloride). The media are stable in short chain alcohols such as ethanol, methanol and propanol, but concentrations above 25% should not normally be used. Note that Sephadex shrinks in alcohol solutions.

Storage

Store unused media 4°C to 30°C in 20% ethanol. Do not freeze.

Wash used media with 2 column volumes of distilled water followed by 2 column volumes of 20% ethanol. Store at 4°C to 30°C.

Alternatively, wash with 2 column volumes of distilled water followed by 2 column volumes 10 mM sodium hydroxide. Sodium hydroxide solution is bacteriostatic, easily disposed of and does not shrink the medium.

Degas the ethanol/water mixture thoroughly and use a low flow rate, checking the back pressure as the column equilibrates.

Avoid changes in temperature, which can cause air bubbles in the packing.

Chapter 6

Sephadex LH-20: size exclusion chromatography in organic solvents

Sephadex LH-20 is specifically designed for the separation and purification of natural products that require the presence of organic solvents to maintain their solubility, including molecules such as steroids, terpenoids, lipids and low molecular weight peptides (up to 35 amino acid residues). Compounds are usually separated by a form of liquid/liquid partitioning or absorption chromatography. Sephadex LH-20 can have a very high selectivity for aromatic compounds in certain solvents and can be used at analytical or industrial scale for the preparation of closely related species. Sephadex LH-20 has found widespread use in the isolation of active components from herb extract used in TCM (Traditional Chinese Medicine).

Sephadex LH-20 is made from hydroxypropylated dextran beads that have been cross-linked to yield a polysaccharide network. The medium can be swollen in water and organic solvents.

Sephadex LH-20 is suitable for an initial purification before polishing by IEX or RPC, or in a final polishing step, for example during the preparation of diastereoisomers.

Sephadex LH-20 exhibits both hydrophilic and hydrophobic properties, the combination of which can offer unique chromatography selectivity for certain applications.



Sephadex has been used for SEC in organic solvents, for example dimethylformamide may be used with Sephadex G-10. Mixtures of water with short-chain alcohols may be used with Sephadex G-10, G-25, and G-50.

Media characteristics

Table 6.1. Characteristics of Sephadex LH-20

Product	Fractionation range (globular proteins)	Sample loading capacity*	Maximum pressure drop over the packed bed	Maximum operating flow rate
Sephadex LH-20	$< 5 \times 10^3$ (exclusion limit will depend on the solvent)	2% of column volume	Solvent-dependent	12 cm/min (720 cm/h, bed height 14 cm, 15 MPa back pressure)

* If Sephadex LH-20 is used in adsorption mode then the sample volume is unlimited until reaching the point of column saturation.

Separation examples

An HIV-1 reverse transcriptase (HIV-1-RT) inhibitor has been isolated from *Phyllanthus niruri*, a natural medicine that has been used for many years to combat edema and jaundice. The active component that inhibits HIV-1 reverse transcriptase has been identified as repandusinic acid A monosodium salt, a small tannin-like molecule. The structure of the free acid is shown in Figure 6.1.

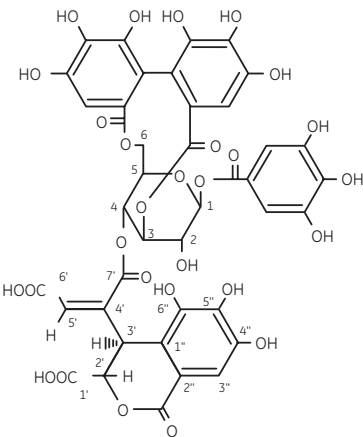


Fig 6.1. Structure of free acid form of repandusinic acid A.

Table 6.2 shows the recovery of active inhibitor from an analytical separation on Sephadex LH-20.

Table 6.2 Summary of data for the isolation of repandusinic acid A from *P. niruri*

Purification step	Yield (mg)	ID ₅₀ * (µg/ml)	Specific activity (× 10 ² IU/mg)	Total activity (× 10 ³ IU) [†]
Water extract	6600	50	4	2640
Methanol insoluble	22 500	20	10	22 500
Sephadex LH-20 fr. 4 to 11 [‡]	247	3.0 to 3.6	56 to 67	11 616
Cellulose				
Fr. 1	189	7.8	26	484
Fr. 2	24	5.0	40	96
Fr. 3	18	2.4	83	150
Fr. 4	9	3.4	58	52
Fr. 5	14	1.8	111	156
RA (pure substance)	5.9	0.3	668	394

* ID₅₀ indicates the effectiveness of inhibitors expressed as concentrations that cause 50% inhibition of HIV-1-RT. Crude HIV-1-RT was used in this experiment.

[†] IU are arbitrary inhibitory activity units obtained by dividing the total weight of the fraction at each step by the weight of each fraction required to achieve 50% inhibition of [³H]dTTP incorporation into the polymer in the HIV-1-RT assay.

[‡] Fractions 4 to 10 and fraction 11 were combined because both fractions had the inhibitory activity.

Figure 6.2 shows Sephadex LH-20 used at a preparative scale for the separation of 2-acetamidobenzoic acid and 4-acetamidobenzoic acid. In this separation the hydrophilicity and hydrophobicity of the medium provide a novel chromatography selectivity resulting in high resolution of closely related species. The molecules differ only by the position of the acetamide moiety on the benzene ring.

Column: Sephadex LH-20, 2.5 × 200 cm
Sample: Mixture of 2- and 4-acetamidobenzoic acid
Eluent: Acetone
Flow rate: 8 ml/min
Detection: Refractive Index (RI)
Yield: 250 mg of 2-acetamidobenzoic acid
 254 mg of 4-acetamidobenzoic acid

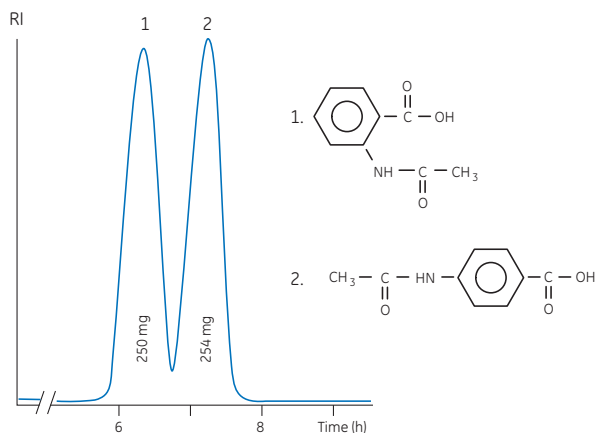


Fig 6.2. Separation of 2- and 4-acetamidobenzoic acid on Sephadex LH-20.

Packing a column

Sephadex LH-20 should be packed in a solvent-resistant (SR) column selected from Table 6.3 according to the column volume required for the separation.

Table 6.3. Sephadex LH-20 packing volumes and bed heights in SR columns

Column	Volume (ml)	Bed height (cm)
SR 25/454	73 to 220	15 to 45
SR 25/100	343 to 490	70 to 100



Simple steps to clarify a sample before applying it to a column will avoid the risk of blockage, reduce the need for stringent washing procedures and extend the life of the chromatography medium. Filter or centrifuge all solvents and samples before use.

1. Refer to Table 6.4 to calculate the amount of dry medium required as the extent of swelling depends upon the solvent system. Swell Sephadex LH-20 for at least 3 h at room temperature in the solvent to be used for the separation.
2. Prepare a slurry 75:25 settled medium:solvent and decant any fine particles of medium.
3. Equilibrate all materials to room temperature.
4. Resuspend and pour the slurry into the column in one continuous step (using a glass rod will help to eliminate air bubbles).
5. Fill the column reservoir to the top with solvent. Seal, attach to a pump, and open the column outlet.
6. Pack at 300 cm/h until the bed has reached a constant height. Stop the flow, empty, and remove the packing reservoir.
7. Carefully fill the column with solvent and insert a wetted adapter into the column. Ensure no air bubbles are trapped under the net and adjust the adapter O-ring to give a sliding seal against the column wall.

8. Connect all tubings, ensuring that there are no air bubbles in the flow path.
9. Slowly slide down the adapter so that any air in the tubings is displaced by solvent and lock the adapter into position on the surface of the medium.
10. Open the column outlet and continue packing until the packed bed is stable and a final adjustment of the top adapter can be made.



In solvents such as chloroform, Sephadex LH-20 is less dense than the solvent and the medium will float. Pour the medium into the column and drain until the second adapter can be inserted. Lock the adapter in position at the surface of the medium and direct the flow of chloroform upwards. The bed will be packed against the top adapter and the lower adapter can be pushed slowly upwards towards the lower surface of the medium. Close the column outlet when moving the adapter to avoid compressing the bed.

Performing a separation

Start at a linear flow of 1 cm/h to check resolution. Low flow rate improves the resolution.

1. Equilibrate the column with at least 2 column volumes of the solvent until a stable baseline is achieved.
2. Apply a sample volume equivalent to 1% to 2% of the total column volume.
3. Elute in 1 column volume. Re-equilibration is not needed between runs with the same solvent.

Cleaning

Wash the column with 2 to 3 column volumes of the solvent, followed by re-equilibration in a new solvent if changing the separation conditions.

Table 6.4. Approximate values for packed bed volumes of Sephadex LH-20 swollen in different solvents

Solvent	Approx. bed volume (ml/g dry Sephadex LH-20)
Dimethyl sulfoxide	4.4 to 4.6
Pyridine	4.2 to 4.4
Water	4.0 to 4.4
Dimethylformamide	4.0 to 4.4
Methanol	3.9 to 4.3
Saline	3.8 to 4.2
Ethylene dichloride	3.8 to 4.1
Chloroform*	3.8 to 4.1
Propanol	3.7 to 4.0
Ethanol†	3.6 to 3.9
Isobutanol	3.6 to 3.9
Formamide	3.6 to 3.9
Methylene dichloride	3.6 to 3.9
Butanol	3.5 to 3.8
Isopropanol	3.3 to 3.6
Tetrahydrofuran	3.3 to 3.6
Dioxane	3.2 to 3.5
Acetone	2.4 to 2.6
Acetonitrile‡	2.2 to 2.4
Carbon tetrachloride‡	1.8 to 2.2
Benzene‡	1.6 to 2.0
Ethyl acetate‡	1.6 to 1.8
Toluene‡	1.5 to 1.6

* Containing 1% ethanol.

† Containing 1% benzene.

‡ Solvents that give a bed volume of less than 2.5 mg/ml dry Sephadex LH-20 are not generally useful.

Chemical stability

Sephadex LH-20 is stable in most aqueous and organic solvent systems. The medium is not stable below pH 2.0 or in strong oxidizing agents.

Storage

Store dry at 4°C to 30°C. Store packed columns and used medium at 4°C to 8°C in the presence of a bacteriostatic agent.

Transferring Sephadex LH-20 from aqueous solution to organic solvents

Transfer Sephadex LH-20 from an aqueous solution to the organic solvent by moving through a graded series of solvent mixtures. This will ensure efficient replacement of the water by the required solvent.

To transfer from aqueous solution or organic solvent (100% A) to a new organic solvent (100% B), proceed as follows: transfer to 70% A:30% B then to 30% A:70% B and finally to 100% B. If A and B are not mutually miscible, make the transfer via an intermediate solvent, for example from water to chloroform via acetone, as shown in Figure 6.3.

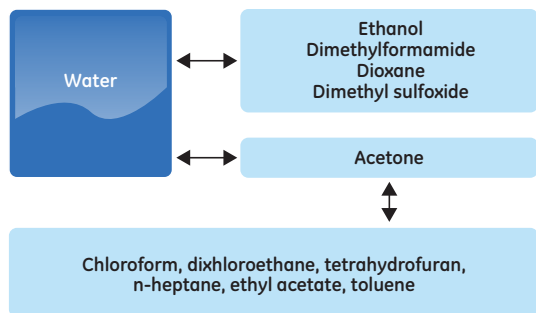


Fig 6.3. Suggested routes for changing to organic solvents.

1. Transfer the required amount of medium to a sintered glass Buchner funnel and remove the excess aqueous solution by gentle suction.
2. Add the next solvent and resuspend the medium by stirring gently.
3. Suck out the excess solvent and resuspend in the same solvent.
4. Repeat the process with the next solvent in the series. Perform at least two resuspensions for each change of solvent conditions until the final solvent composition is reached.
5. Pack the medium into solvent resistant SR 25/45 or SR 25/100 columns.

Chapter 7

Size exclusion chromatography in theory

Defining the process

Results from SEC are usually expressed as an elution profile or chromatogram that shows the variation in concentration (typically in terms of UV absorbance, for proteins usually at 280 nm) of sample components as they elute from the column in order of their molecular size. Figure 7.1 shows a theoretical chromatogram of a high-resolution fractionation. Molecules that do not enter the matrix are eluted together in the void volume, V_0 , as they pass directly through the column at the same speed as the flow of buffer. For a well-packed column, the void volume is equivalent to approximately 30% of the total column volume. Molecules with partial access to the pores of the matrix elute from the column in order of decreasing size. Small molecules such as salts that have full access to the pores move down the column, but do not separate from each other. These molecules usually elute just before one total column volume, V_t , of buffer has passed through the column.

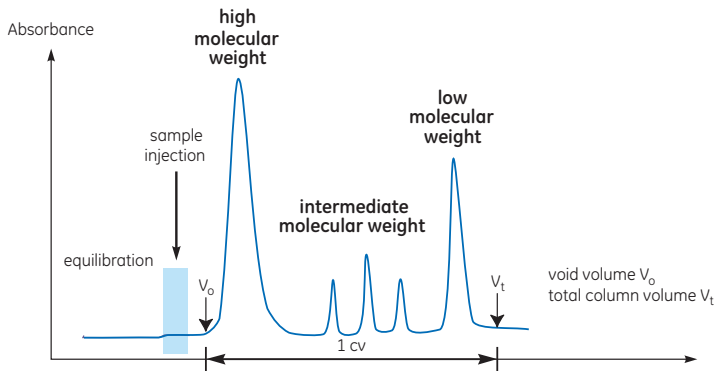


Fig 7.1. Theoretical chromatogram of a high-resolution fractionation.

The behavior of each component can be expressed in terms of its elution volume, V_e from the chromatogram. As shown in Figure 7.2, there are three different ways of measuring V_e , dependent on the volume of sample applied to the column. V_e is the direct observation of the elution properties of a certain component.

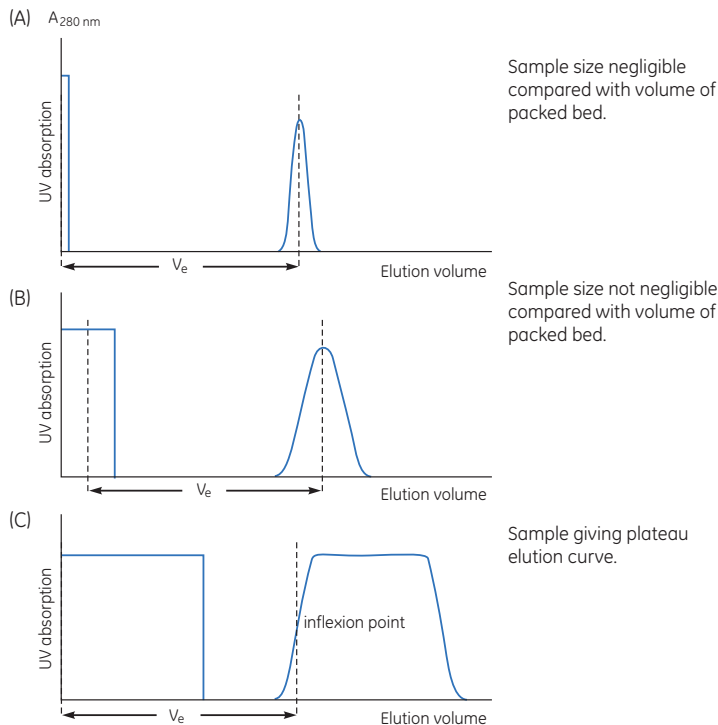


Fig 7.2. Measurement of elution volume, V_e . (A) Sample size negligible compared with volume of packed bed. (B) Sample size not negligible compared with volume of packed bed. (C) Sample giving plateau elution curve.

Since symmetrical peaks are common in SEC, elution volumes are easily determined. However, V_e will vary with the total volume of the packed bed (V_t) and the way in which the column has been packed. The elution of a sample is best characterized by a distribution coefficient (K_d). K_d is used for column comparison since it is independent of column dimensions and thus allows comparison and prediction between columns with different sizes if the same medium and sample is used.

K_d is derived as follows:

The volume of the mobile phase (buffer) is equal to the void volume, V_o . The void volume, V_o is the elution volume of molecules that remain in the buffer because they are larger than the largest pores in the matrix and therefore pass straight through the packed bed (Fig 7.3). In a well-packed column, the void volume is approximately 30% of the total physical volume.

The volume of the stationary phase, V_s , is equal to V_i , the volume of buffer inside the matrix. This volume is available only to very small molecules. V_i is the elution volume of molecules that distribute freely between the mobile and stationary phases minus the void volume. K_d represents the fraction of the stationary phase that is available for diffusion of a given molecular species:

$$K_d = \frac{V_e - V_o}{V_t - V_o - V_{\text{gel matrix}}} = \frac{V_e - V_o}{V_i}$$

Since, in practice, V_s or V_i are difficult to determine, it is more convenient to employ the term $(V_t - V_o)$. The estimated volume of the stationary phase will therefore include the volume of solid material which forms the matrix.

The stationary phase volume V_s can be substituted by the term $(V_t - V_o)$ in order to obtain a value K_{av} .

$$K_{av} = (V_e - V_o) / (V_t - V_o)$$

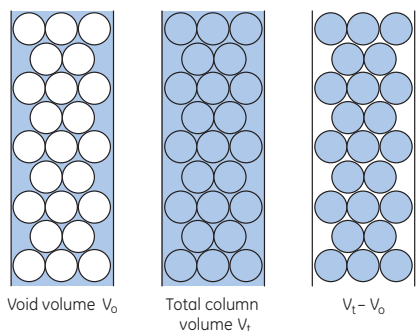


Fig 7.3. Diagrammatic representation of V_t and V_0 . Note that $V_t - V_0$ will include the volume of the solid material which forms the matrix (Fischer, L. Laboratory Techniques in Biochemistry and Molecular Biology. Vol. 1 part II. An Introduction to Gel Chromatography. North Holland Publishing Company, Amsterdam. Reproduced by kind permission of the author and publisher).

Since $(V_t - V_0)$ includes the volume of the matrix that is inaccessible to all solute molecules, K_{av} is not a true partition coefficient. However, for a given medium there is a constant ratio of $K_{av}:K_d$ which is independent of the nature of the molecule or its concentration. K_{av} is easily determined and, like K_d , defines sample behavior independently of the column dimensions and packing. Other methods of normalizing data give values that vary depending upon how well the column is packed. The approximate relationships between some of these terms are shown in Figure 7.4.


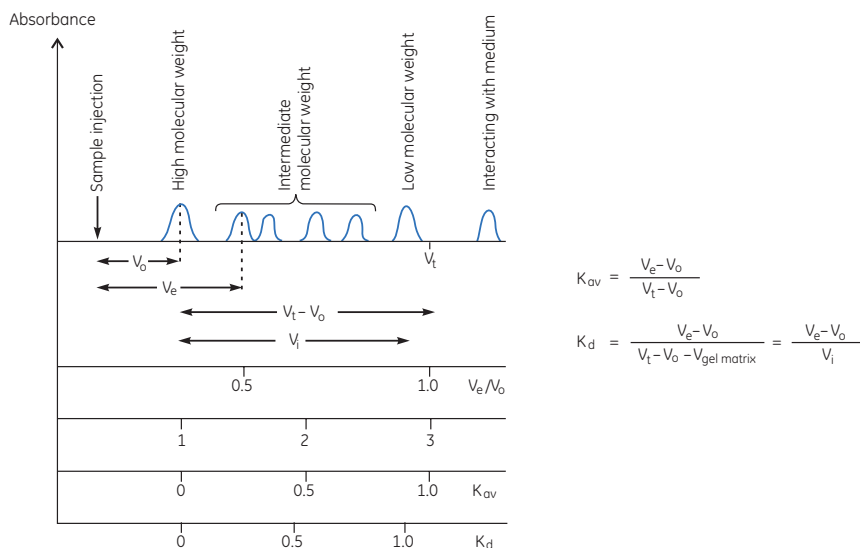


Fig 7.4. Relationship between several expressions used for normalizing elution behavior.


Selectivity curves and media selection

The partition coefficient K_{av} is related to the size of a molecule. Molecules of similar shape and density demonstrate a sigmoidal relationship between their K_{av} values and the logarithms of their molecular weights (M_r). Over a considerable range there is a virtually linear relationship between K_{av} and $\log M_r$. The selectivity of a SEC medium depends solely on its pore size distribution and is described by a selectivity curve. By plotting K_{av} against the log of the molecular weight for a set of standard proteins, selectivity curves are created for each SEC medium, as shown in Figure 7.5.

Superdex 30 prep grade

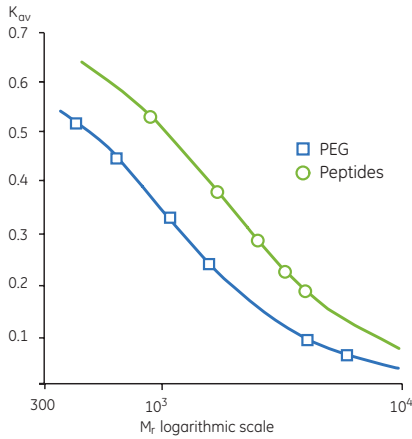

Superdex 75 prep grade and Superdex 200 prep grade

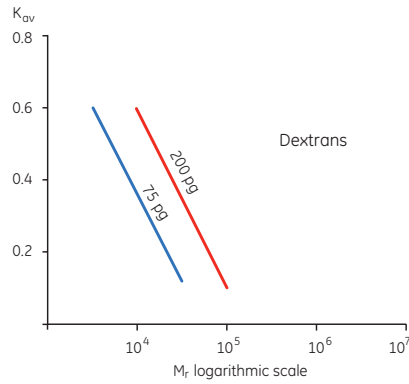

Superdex 75 prep grade and Superdex 200 prep grade

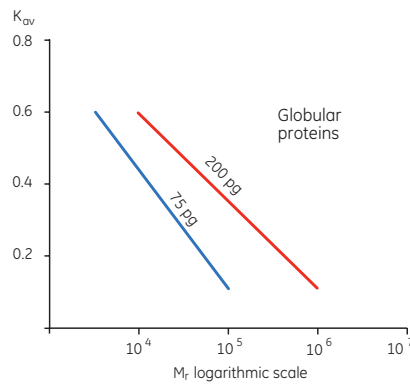


Fig 7.5. Selectivity curves for Superdex 30 prep grade, Superdex 75 prep grade, and Superdex 200 prep grade.

SEC media should be selected so that the important components are found in the most linear part of the selectivity curve with minimum peak broadening or dilution and minimum time on the column. The lowest molecular weight substances should be eluted near V_t ($K_{av} = 1$).



Under optimal conditions, no molecules can be eluted with a K_{av} greater than 1 or less than 0.



If the K_{av} is greater than 1, molecules have bound nonspecifically to the chromatographic medium.



If K_{av} is less than 0 after calibration, there is channeling in the chromatography bed and the column must be repacked.



The steeper the selectivity curve, the higher the resolution that can be achieved.

Resolution

Resolution (R_s) is defined by the following expression:

$$R_s = \frac{V_{e2} - V_{e1}}{\frac{(W_1 + W_2)}{2}}$$

V_{e1} and V_{e2} are the elution volumes for two adjacent peaks measured at the center of the peak. W_1 and W_2 are the respective peak widths.

V_{e1} and V_{e2} are the elution volumes for two adjacent peaks measured at the center of the peak. W_1 and W_2 are the respective peak widths. $(V_{e2} - V_{e1})$ represents the distance between the peaks and $1/2 (W_1 + W_2)$ the mean peak width of the two peaks as shown in Figure 7.6.

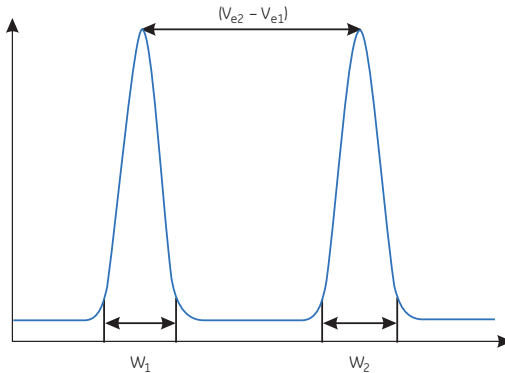


Fig 7.6. Parameters used to define resolution (R_s).

Final resolution, the degree of separation between peaks, is influenced by many factors: the ratio of sample volume to column volume, flow rate, column dimensions, particle size, particle size distribution, packing density, porosity of the particle, and viscosity of the mobile phase. The success of SEC depends primarily on choosing conditions that give sufficient selectivity and counteract peak broadening effects during the separation.

Resolution is a function of the selectivity of the medium and the efficiency of that medium to produce narrow peaks (minimal peak broadening) as illustrated in Figure 7.7.

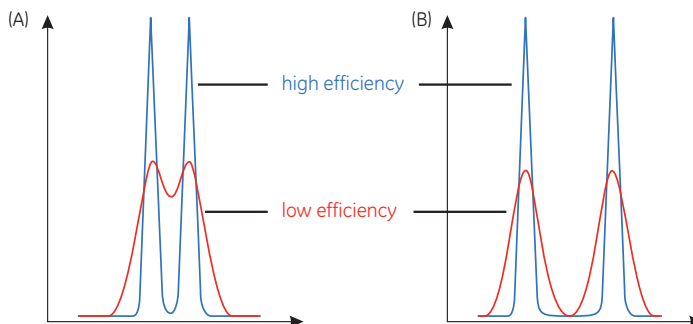


Fig 7.7. Resolution depends on the selectivity of the media and the counteraction of peak broadening (lower efficiency). (A) Good resolution (blue curve) and poor resolution (red curve). (B) Excellent resolution (blue curve) and good resolution (red curve).

The homogeneity of the packed bed and the particles influences the uniformity of the flow through the column and hence affects the shape and eventual peak width. SEC media with high uniformity and narrow particle size distribution facilitate the elution of molecules in sharp peaks.

SEC media with smaller particle sizes facilitate diffusion of sample molecules in and out of the particles by reducing the time to achieve equilibrium between mobile and stationary phases and so improve resolution by reducing peak width.

Sample dilution is inevitable because diffusion occurs. In order to minimize sample dilution, a maximum sample volume is used within the limits set by the separation distance, that is, the resolution required between the peaks of interest. The sample can be regarded as a zone passing down the column. Figure 7.8 shows how, if no zone broadening occurs, the maximum sample volume could be as great as the separation volume (V_{sep}):

$$V_{sep} = V_{eB} - V_{eA}$$

However, due to eddy diffusion, nonequilibrium between the stationary phase and the buffer, and longitudinal diffusion in the bed, the zones will always be broadened. Therefore the sample volume must always be smaller than the separation volume.

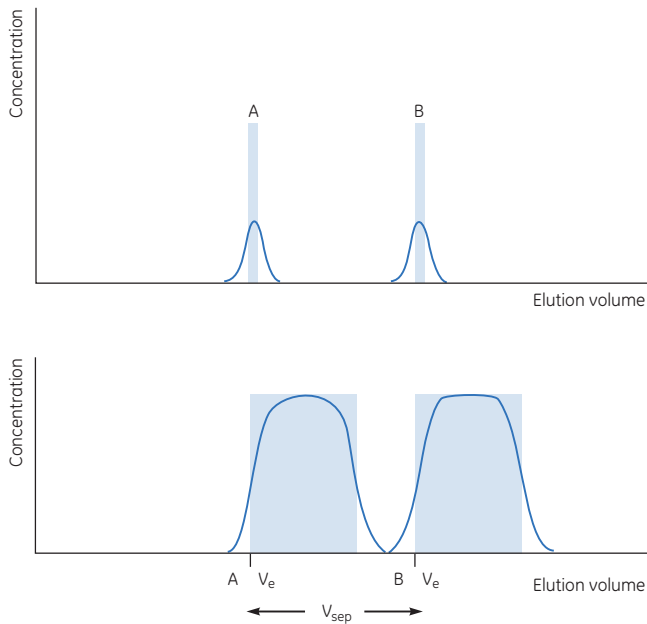


Fig 7.8. Elution curves for different sample sizes. The top diagram corresponds to the application of a small sample. The bottom diagram corresponds to the maximum sample volume to obtain complete separation in the conditions of the experiment. The shaded areas correspond to the elution profiles that would be obtained if there was no zone broadening.

Chapter 8

Size exclusion chromatography in a purification strategy

The three-phase purification strategy of Capture, Intermediate Purification, and Polishing (CIPP) is used in both the pharmaceutical industry and in the research laboratory to ensure faster method development, a shorter time to pure product, and good economy. This chapter gives a brief overview of this approach, which is recommended for any multistep protein purification. The *Strategies for protein purification handbook*, code number 28-9833-31 from GE Healthcare is recommended as a guide to planning efficient and effective protein-purification strategies.

As shown in Figure 8.1, an important first step for any purification is correct sample preparation and this is covered in more detail in Appendix 3. SEC is often used for desalting and buffer exchange during sample preparation using Sephadex G-25, and samples volumes up to 30% of the total column volume can be applied.

In high-resolution mode, SEC is an excellent choice for the final polishing steps in a purification when sample volumes have been reduced (sample volume significantly influences speed and resolution in SEC). Samples are eluted isocratically (single buffer, no gradient) and buffer conditions can be varied to suit the sample type or the requirements for subsequent purification, analysis or storage, since buffer composition does not directly affect resolution.

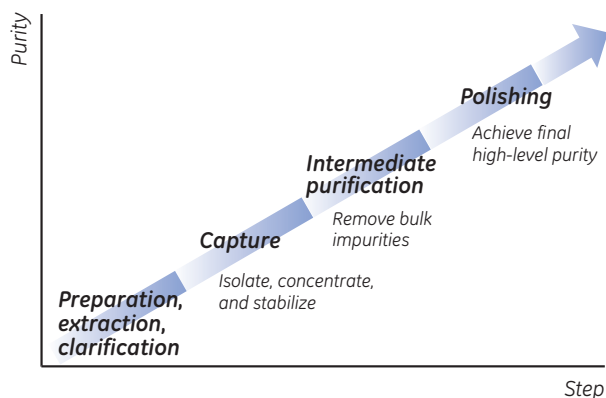


Fig 8.1. Sample preparation and CIPP purification strategy.

The purification strategy according to CIPP



Imagine the purification has three phases: Capture, Intermediate Purification, and Polishing. Each phase can include one or more purification steps.



Assign a specific objective to each step within the purification process.

The problem associated with a particular purification step will depend greatly upon the properties of the starting material. Thus, the objective of a purification step will vary according to its position in the process.

In the capture phase, the objectives are to isolate, concentrate, and stabilize the target product. The product should be concentrated and transferred to an environment that will conserve potency/activity.

During the intermediate purification phase, the objective is to remove most of the bulk impurities, such as other proteins, nucleic acids, endotoxins, and viruses.

In the polishing phase, most impurities have already been removed except for trace amounts or closely related substances. The objective is to achieve final purity by removing any remaining trace impurities or closely related substances.

 The optimal selection and combination of purification techniques for Capture, Intermediate Purification, and Polishing is crucial for an efficient purification.

A guide describing the main features of the most common purification techniques and their use in the different phases in CIPP is shown in Table 8.1.

Table 8.1. Properties of different purification techniques and strategies for their use in CIPP

Method	Typical characteristics		Purification phase			Sample start conditions	Sample end conditions
	Resolution	Capacity	Capture	Intermediate	Polishing		
AC	+++ or ++	+++ or ++	+++	++	+	Various binding conditions	Specific elution conditions
IMAC	+++	++	+++	++	+	For purifying histidine-tagged proteins using Ni Sepharose prepacked columns: 20 to 40 mM imidazole, pH > 7, 500 mM sodium chloride; no chelators Other proteins: low concentration of imidazole	High concentration of imidazole, pH > 7, 500 mM sodium chloride
SEC	++	+	+		+++	Most conditions acceptable, limited sample volume	Buffer exchange possible. Diluted sample
IEX	+++	+++	+++	+++	+++	Low ionic strength. pH depending on protein and IEX type	High ionic strength or pH changed
HIC	+++	++	++	+++	+++	High ionic strength. Addition of salt required	Low ionic strength
Chromato-focusing (CF)	+++	+			++	Low ionic strength	Polybuffer. Low ionic strength
RPC	+++	++		+	++	Ion-pair reagents and organic modifiers might be required	Organic solvents (risk for loss of biological activity)

SEC as a polishing step

Most commonly, separations by charge, hydrophobicity, or affinity will have been used in earlier stages of a purification strategy so that high-resolution SEC is a good choice for the final polishing step. The product can be purified and transferred into the required buffer in one step and dimers and aggregates can be removed, as shown in Figure 8.2.

SEC is also the slowest of the chromatography techniques and the size of the column determines the volume of sample that can be applied. It is therefore most logical to use SEC after techniques that reduce sample volume so that smaller columns can be used.

Column: XK 16/60 packed with Superdex 75 prep grade
 Sample: Partly purified ZZ-brain IGF
 Sample load: 1.0 ml
 Buffer: 300 mM ammonium 0.5 ml/min
 Flow rate: 0.5 ml/min (15 cm/h)

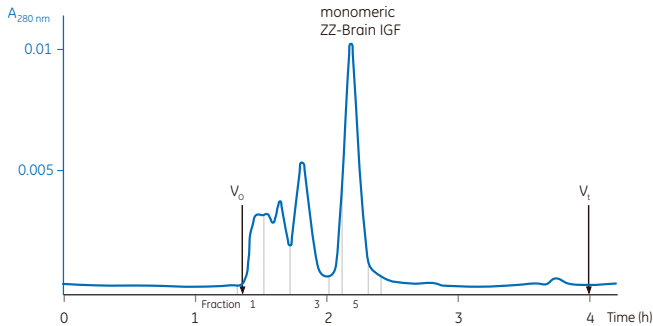


Fig 8.2. Final polishing step: separation of dimers and multimers on Superdex 75 prep grade.



Media for polishing steps should offer the highest possible resolution. Superdex is the first choice at laboratory scale and Superdex prep grade for large-scale applications.

CIPP does not mean that there must always be three purification steps. For example, capture and intermediate purification might be achievable in a single step, as might intermediate purification and polishing. Similarly, purity demands can be so low that a rapid capture step is sufficient to achieve the desired result. For purification of therapeutic proteins, a fourth or fifth purification step might be required to fulfill the highest purity and safety demands. The number of steps used will always depend upon the purity requirements and intended use for the protein.

Purification of humanized IgG₄ monoclonal antibody

A humanized IgG₄ monoclonal antibody was expressed in a myeloma cell culture and purified by a combination of AC and SEC (Fig 8.3). The antibody was captured by AC using MabSelect™. SEC on HiLoad Superdex 200 pg column was then used to separate the monomer from the dimer and larger polymers.





Capture by affinity chromatography

Column: MabSelect (18 ml), XK 16/20 column
Sample: 1282 ml of myeloma cell culture containing humanized IgG₄ (~0.33 mg/ml)
Binding buffer: 20 mM sodium phosphate, 150 mM sodium chloride, pH 7.4
Elution buffer: 100 mM sodium citrate, pH 3.0
Flow rate: 220 cm/h (7.4 ml/min)
Operation: Equilibration: 5 column volumes (CV) of binding buffer
 Sample application: 1282 ml.
 Wash: 10 CV of binding buffer.
 Elution: step gradient 100%, 5 CV of elution buffer

Purification of the monomer (polishing step)

Column: HiLoad 26/60 Superdex 200 prep
Sample: 7.5 ml of the pooled fractions from MabSelect column
grade
Buffer: 50 mM sodium phosphate, 150 mM sodium chloride, pH 7.0
Flow rate: 22.6 cm/h (2 ml/min)
Operation: Equilibration 2 CV, Sample application, Isocratic elution 1 CV

CV = total column volume = V_t

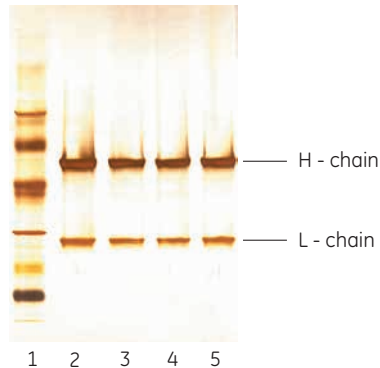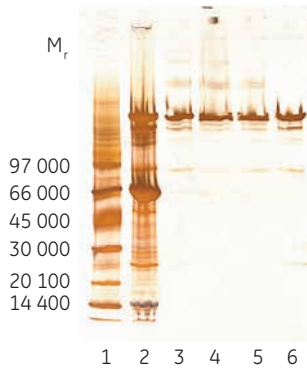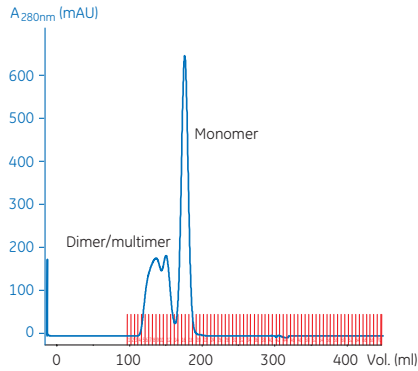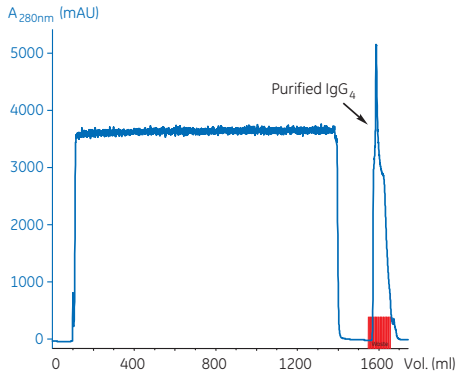

Analysis: SDS-PAGE, silver staining

Unreduced sample

Lanes

1. LMW Marker
2. Crude sample from myeloma cell culture
3. Pooled eluted sample from capture step
4. Fraction 4 to 9 from polishing step
5. Fraction 10 to 12 from polishing step
6. Fraction 14 to 18 from polishing step

Reduced sample

1. LMW Marker
2. Pooled eluted sample from capture step
3. Fraction 4 to 9 from polishing step
4. Fraction 10 to 12 from polishing step
5. Fraction 14 to 18 from polishing step

Fig 8.3. Two-step purification of humanized IgG₄. Affinity chromatography was used for the first step while SEC was used for the second step in the purification.

Appendix 1

Column packing and preparation

A well-packed column is essential for a high-resolution fractionation on any SEC medium. Prepacked columns from GE Healthcare will ensure reproducible results and the highest performance. If the column volume or medium you require is not available as a prepacked column, contact your local GE Healthcare sales representative to inquire about our column packing services.

Packing a column is a very critical stage in any SEC experiment. A poorly packed column will give rise to uneven flow, peak broadening, and loss of resolution. It can also affect achievable flow rates. If you decide to pack an SEC column yourself then the guidelines in this appendix will apply at any scale of operation.

An instructive video on a CD, is available to demonstrate how to produce a well-packed column (see Ordering information for *Column Packing to The Movie*). It focuses particularly on the importance of column packing for gel filtration. SEC is simple to perform once a well-packed column has been obtained. Providing that a column is used and maintained carefully it can be expected to give reproducible, high-resolution results for a long time.



Ensure that there is sufficient buffer for long, unattended runs or that the pump is programmed to stop the flow after a suitable time. SEC columns that run dry must be repacked.

Columns for packing SEC media

Empty columns from GE Healthcare are fully compatible with the high flow rates achievable with modern media and a broad range of column dimensions is available. Ordering information for empty columns and main accessories can be found at the back of this handbook.

Table A1.1. Maximum bed heights (cm) and bed volumes (ml) using one or two adapters in XK columns

Column	With one adapter		With two adapters	
	Volume (ml)	Bed height (cm)	Volume (ml)	Bed height (cm)
XK 16/20	5 to 31	2.5 to 15.5	0 to 31	0 to 15.5
XK 16/40	45 to 70	22.5 to 35	16 to 70	8 to 35
XK 16/70	105 to 130	52.5 to 65	76 to 130	38 to 65
XK 16/100	165 to 190	82.5 to 95	136 to 190	68 to 95
XK 26/20	5 to 66	1 to 12.5	0 to 66	0 to 12.5
XK 26/40	122 to 186	23 to 35	45 to 186	8.5 to 35
XK 26/70	281 to 344	53 to 65	204 to 344	38.5 to 65
XK 26/100	440 to 504	83 to 95	365 to 504	68.5 to 95
XK 50/20	0 to 274	0 to 14	0 to 274	0 to 14
XK 50/30	265 to 559	14 to 28	0 to 559	0 to 28
XK 50/60	794 to 1088	40 to 56	500 to 1088	26 to 56
XK 50/100	1588 to 1862	81 to 95	1274 to 1862	65 to 95

Adapters are adjustable column end pieces that help to eliminate any disturbances to the surface of the packed medium as sample is applied and to prevent insoluble particles from entering and blocking the column.


Tricorn and XK empty columns are delivered with one adapter, but a second adapter can be used instead of a column end piece if a shorter bed height is required. HiScale™ columns are equipped with dual adapters. A range of accessories are available for all empty columns.

Table A1.2. Bed volumes and heights for Tricorn columns

Bed volumes and heights		With one adapter		With two adapters	
		Volume (ml)	Bed height (mm)	Volume (ml)	Bed height (mm)
Tricorn Column	Column i.d. (mm)				
Tricorn 10/20	10	0.00 to 2.29	0 to 29	0.00 to 2.07	0 to 26
Tricorn 10/100	10	6.21 to 8.57	79 to 109	3.64 to 8.36	46 to 106
Tricorn 10/150	10	10.14 to 12.50	129 to 159	7.57 to 12.28	96 to 156
Tricorn 10/200	10	14.07 to 16.42	179 to 209	11.50 to 16.21	146 to 206
Tricorn 10/300	10	21.92 to 24.28	279 to 309	19.35 to 24.06	246 to 306
Tricorn 10/600	10	45.48 to 47.84	579 to 609	42.91 to 47.63	546 to 606

Table A1.3. Bed heights and volumes for HiScale columns

Column	Max. column bed height (cm), max. column volume (ml) with one adapter
HiScale 16/20	20 cm, 40 ml
HiScale 26/20	20 cm, 106 ml
HiScale 16/40	40 cm, 80 ml
HiScale 26/40	20 cm, 212 ml
HiScale 50/20	20 cm, 393 ml
HiScale 50/40	20 cm, 785 ml

 Longer columns (50 cm and more) can be difficult to pack under normal laboratory conditions. As alternatives, use our column packing services or connect two or more shorter columns (20 or 30 cm bed height) in series to achieve the required bed height.

Checking column efficiency

Column performance should be checked at regular intervals by determining the theoretical plate number and peak symmetry. Note that the result for column efficiency is dependent on the system used, including the capillaries and dead volumes. This means that the column efficiency given in the specification for the column (tested on another system) will not be the same as your initial column efficiency result.

Typical values for column performance:

Superdex prep grade: Efficiency $N/m > 10\,000$, Peak symmetry $A_s = 0.70$ to 1.30

Sephacryl HR: Efficiency $N/m < 9000$, Peak symmetry $A_s = 0.80$ to 1.50

1. Equilibrate the packed column in distilled water at the recommended flow rate given in the instructions.
2. Inject acetone (20 mg/ml in water) in a volume equivalent to 0.2% of the total packed column volume.
3. Monitor UV absorbance 280 nm from the time of injection until the acetone peak has eluted and the signal has returned to baseline.
4. Calculate column efficiency, that is, the number of theoretical plates per meter (N/m):

$$N/m = 5.54 (V_e / W_{1/2})^2 / L$$

where

V_e = peak elution (retention) volume

$W_{1/2}$ = peak width at half peak height

L = bed height (m)

V_e and $W_{1/2}$ are in same units

Calculate the asymmetry factor (A_s):

$$A_s = b/a$$

where

a = first half peak width at 10% peak height

b = second half peak width at 10% peak height

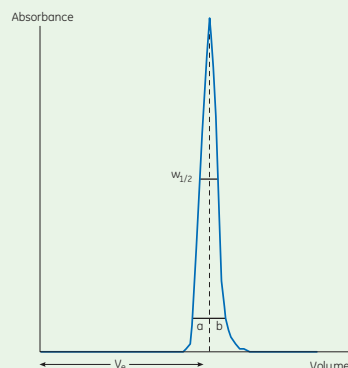


Fig A1.1. Determination of column efficiency by number of theoretical plates and peak symmetry.

Column packing for high-resolution fractionation using Superdex prep grade and Sephacryl High Resolution

Superdex prep grade and Sephacryl High Resolution media should be packed and equilibrated at high flow rate using a column from the XK-series. XK columns are optimally designed for SEC with a bed design that ensures a uniform liquid flow and a dead space at the column outlet of less than 0.1% of the column volume in order to minimize dilution and to prevent remixing of separated peaks. XK columns are manufactured from materials that do not interfere with labile biological substances. They are easy to dismantle and reassemble for thorough cleaning, which is particularly important when handling biological samples.



Ensure that the column and all components are clean and in good condition. It is particularly importance that the nets, net fasteners, and glass tube are not damaged. Use well degassed buffers and equilibrate all materials to the temperature at which the separation will be performed. Avoid columns with large dead volumes as this will affect resolution.



For high-resolution fractionation, use bed heights between 30 and 60 cm. Apply sample volumes equivalent to between 1% and 2% of the column volume. The sample volume can be increased up to 4% if resolution in the particular application is good enough.



The settled medium should have a volume of 1.15-fold that of the required packed column volume, see Table A1.1 to A1.3 for examples.

1. Superdex prep grade and Sephacryl HR are supplied swollen in a suspension containing 20% ethanol as a preservative. Suspend the medium by shaking gently and pour a sufficient quantity into a graduated glass cylinder or beaker.



Avoid using magnetic stirrers, spatulas or glass rods since they can damage the matrix.

2. Wash the medium with 5 to 10 column volumes of distilled water on a glass filter and resuspend in distilled water to a final concentration of 50% settled medium. The medium must be thoroughly washed to remove the 20% ethanol storage solution. Residual ethanol can interfere with subsequent procedures.



To produce a more evenly dispersed slurry of Superdex prep grade, Tween™ 20 (250 ml per 500 ml washed slurry) can be added in order to reduce surface tension.

3. Wet the bottom filter by injecting distilled water through the effluent tubing. Close the end piece outlet. Mount filter and bottom end piece onto the column.

4. Attach the packing reservoir tightly to the column.



For XK 16 and XK 26 columns using a second column instead of a packing reservoir makes it easier to obtain a well-packed column. The second column is used with Packing Connector XK 16 or XK 26 as appropriate.

5. Mount the column and packing reservoir vertically on a laboratory stand.
6. Fill the column with distilled water to a height of 2 cm above the column end piece. Avoid air bubbles.
7. Degas the suspended medium under vacuum and carefully pour the suspended medium down the wall of the column using a glass rod. Avoid introducing air bubbles. Pour everything in a single operation and fill the reservoir to the top with distilled water.
8. Connect the pump outlet to the inlet on the packing reservoir. Open the column outlet and start the flow of buffer, see Table A1.4 for flow recommendations.



To achieve satisfactory column efficiency, Superdex prep grade must be packed in two steps: Step 1 for 2 h or until the bed has reached a constant height and Step 2 for 60 min. Table A1.4 shows the flow rates for each step.



Sephacryl HR can usually be packed satisfactorily using only the higher flow rate given in Step 2 of Table A1.4. Use the two step process if the column efficiency was unsatisfactory after the first attempt.

9. Stop the pump and remove the packing reservoir. Carefully fill the column with distilled water to form an upward meniscus at the top and insert the adapter. Adjust the adapter to the surface of the packed bed.
10. Continue packing the column at the flow rate used in Step 2 for approximately 10 min. If the recommended flow rate cannot be obtained, use the maximum flow rate the pump can deliver. Mark the position of the top of the packed medium, stop the pump, close the column outlet, move the adapter down onto the surface of the medium and then push the adapter a further 3 mm into the medium. The column is now ready to use. See Table A1.4 for maximum recommended flow rate and operating pressure for Sephacryl HR and Superdex prep grade media.



Do not exceed maximum pressures during packing: 0.2 to 0.4 MPa, 2 to 4 bar for Sephacryl S-300 HR and S-100 HR respectively, 0.15 MPa, 1.5 bar for Sephacryl S-400 HR and S-500 HR, and 0.4 to 0.5 MPa, 4 to 5 bar for Superdex prep grade (75 and 200).



Always check the specific storage instructions supplied with the product.

Table A1.4. Recommended flow rates during column packing

Column	Bed height (cm)	Step 1 Sephacryl HR (ml/min)	Step 2 Sephacryl HR (ml/min)	Step 1 Superdex prep grade (ml/min)	Step 2 Superdex prep grade (ml/min)
XK 16/40	35	1 to 2	2 to 4	1 to 2	4 to 6
XK 16/70	65	1 to 2	2 to 4	1 to 2	4 to 6
XK16/100	95	1 to 2	2 to 4	1 to 2	4 to 6
XK 26/40	35	2 to 4	4 to 8	2 to 4	10 to 14
XK 26/70	65	2 to 4	4 to 8	2 to 4	10 to 14
XK 26/100	95	2 to 4	4 to 8	2 to 4	10 to 14
XK 50/20	10 to 15	8 to 10	4 to 8	9 to 11	19 to 21
XK 50/30	20 to 25	8 to 10	4 to 8	9 to 11	19 to 21
XK 50/60	55	8 to 10	4 to 8	9 to 11	19 to 21
XK 50/100	95	8 to 10	4 to 8	9 to 11	19 to 21

Column packing for group separations using Sephadex

Sephadex is supplied as a dry powder and must be allowed to swell in excess buffer before use. After swelling, adjust with buffer to form a thick slurry from which air bubbles are removed under vacuum. Approximately 75% settled medium is suitable. Fine particles can be decanted.



Accelerate the swelling process by using a boiling water bath (Table A1.5). This also serves to degas the suspension. Allow the suspension to cool before use.

Table A1.5. Bed volume and swelling times for Sephadex

Medium	Approx. bed volume (ml/1 g medium)	Swelling time (h), 20°C	Swelling time (h), 90°C
Sephadex G-10 Medium	2 to 3	3	1
Sephadex G-25 (all grades)	4 to 6	3	1
Sephadex G-50 Fine	9 to 11	3	1



Ensure that the column and all components are clean and in good condition. It is particularly important that the nets, net fasteners, and glass tube are not damaged. Use well-degassed buffers and equilibrate all materials to the temperature at which the separation will be performed. Keep a packed column away from locations that are exposed to drafts or direct sunlight that can cause temperature changes and the formation of bubbles.



For group separations, use up to 10 cm bed height. Sample volumes can be up to 30% of the column volume. Pack a quantity of medium up to five-fold the volume of the sample to be desalted.

Note: These instructions assume that a column with two adapters is used for packing.

1. Weigh out the correct amount of dry Sephadex and allow the medium to swell according to the instructions above. Avoid using magnetic stirrers, spatulas, or glass rods since they can damage the medium.
2. Wet the bottom filter by injecting distilled water through the effluent tubing. Close the end piece outlet. Mount filter and bottom end piece onto the column.

3. If the slurry volume is greater than the volume of the column, attach a packing reservoir to the column.
4. Mount the column and packing reservoir vertically on a laboratory stand.
5. Fill the column with distilled water or buffer to a height of approximately 2 cm above the column end piece. Avoid air bubbles.
6. Pour the well-mixed and well-degassed suspension in a single operation down the inside wall using a glass rod. Avoid introducing air bubbles.
7. Connect the pump outlet to the inlet of the packing reservoir. Open the column outlet and start the flow of buffer. Pass 2 to 3 column volumes of buffer through the column in order to stabilize the bed and equilibrate completely. Use a slightly higher flow rate than the flow rate to be used during separations.
8. Maintain the packing flow rate for at least 3 column volumes after a constant bed height is obtained.
9. Mark the bed height on the column and close the column outlet. Remove the packing reservoir.
10. Add buffer carefully to fill the column and form an upward meniscus.
11. Connect all tubings. Slacken the adapter tightening mechanism and insert the adapter at an angle into the column so that no air is trapped under the net. Slide the adapter slowly down the column until the mark is reached. Note that the outlet of the adapter should be open and the column outlet should be closed.
12. Adjust the tightening mechanism to give a sliding seal between the column wall and O-ring. Screw the adapter onto the column.
13. Continue packing the column for approximately 10 min. Stop the pump, close the column outlet, and move the top adapter down onto the surface of the medium. Push the adapter a further 3 mm into the medium. The column is now ready for equilibration.

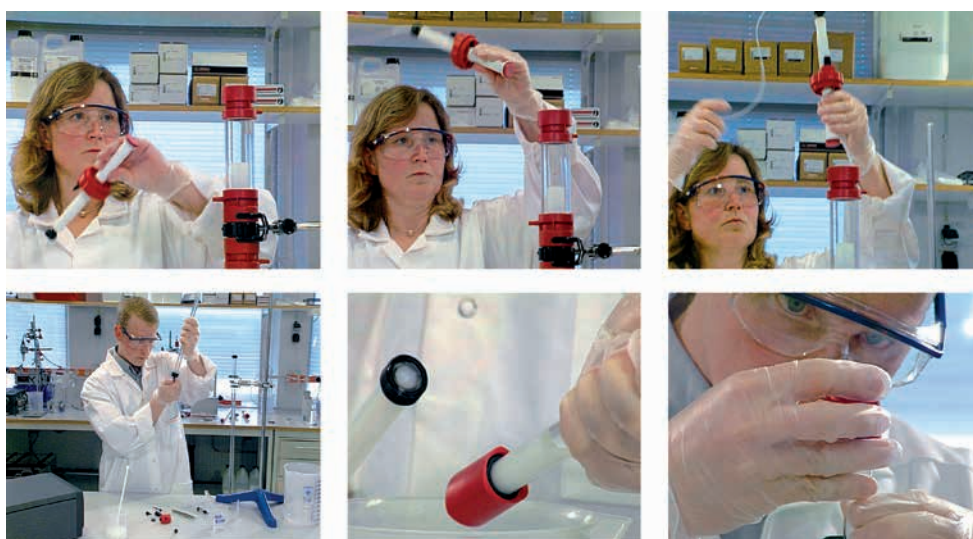


Fig A1.2. *Column Packing — The Movie* provides a step-by-step demonstration of column packing.



Sephadex G-10, G-25, and G-50 obey Darcy's law, that is, if the flow rate is doubled then the column pressure will double, hence maximum values for flow rates or operating pressures do not need to be considered (see Appendix 2 for an explanation of Darcy's law).

Controlling flow rates

The safest and easiest way in which to control flow rates during column packing and chromatography separation is to use a pump controlled within an ÄKTA chromatography system. Accurate and reproducible flow control is particularly important for efficient column packing and when repeating experiments or performing routine preparative work. A peristaltic pump can be used with Sephadex packed in smaller columns.



The maximum flow rate achievable will depend on column diameter and buffer viscosity. Narrow columns allow a higher pressure and higher linear flow (cm/h) than wide columns.



Always connect a pump so that buffer is pumped onto the column (rather than connecting the pump after the column and drawing buffer through the column). This reduces the risk of bubble formation due to suction effects.



Always use a flow rate for column packing that is higher than the flow rate used for separation.



Do not exceed the maximum recommended values for pressure or linear flow for the medium. Exceeding these values might cause the medium to compress and reduce the flow rate and resolution during the separation.



Do not exceed 75% of the packing flow rate during any separation.



Do not use a peristaltic pump when packing Superdex or Sephacryl media in larger columns since a flow rate high enough to obtain high-resolution fractionation cannot be achieved.

Appendix 2

Sephadex and Darcy’s law

Sephadex G-10, G-25, and G-50 can be assumed to behave as rigid spheres in SEC and therefore obey Darcy’s Law. This Law describes a general relationship for flow in porous media:

$$U = K \times \Delta P \times L^{-1}$$



Equation (1)

- U = linear flow rate expressed in cm/h (see Appendix 5)
- ΔP = pressure drop over the packed bed expressed in cm water
- L = bed height expressed in cm
- K = constant of proportionality depending on the properties of the bed material and the buffer

Assuming a buffer with viscosity of 1 cP: $U = K_o \times \Delta P \times L^{-1}$

Equation (2)

K_o = the “specific permeability” depending on the particle size of the medium and the water regain

-  Note that flow is proportional to the pressure drop over the bed and, assuming a constant pressure head, inversely proportional to the bed height. In practice this means that the pressure/flow considerations that must be made when using other SEC media do not apply to Sephadex and that a doubling of flow rate leads to a doubling in column pressure. To a good approximation, flow rate is independent of the column diameter.
-  Flow at viscosities greater than 1 cP can be obtained by using the relationship: flow rate is inversely proportional to viscosity. High buffer viscosities can be compensated for by increasing the operating pressure to maintain a high flow rate.

Theoretical flow (not maximum) can be calculated from equation (2) by inserting values for ΔP and L. Specific permeabilities (K) are given in Table A2.1.

Table A2.1. Specific permeabilities of Sephadex

Sephadex type	Permeability K
Sephadex G-10	19
Sephadex G-25 Superfine	9
Sephadex G-25 Fine	30
Sephadex G-25 Medium	80
Sephadex G-25 Coarse	290
Sephadex G-50 Fine	36

Appendix 3

Sample preparation

Samples for chromatographic purification should be clear and free from particulate matter. Simple steps to clarify a sample before beginning purification will avoid clogging the column, can reduce the need for stringent washing procedures, and can extend the life of the chromatographic medium.

Sample extraction procedures and the selection of buffers, additives, and detergents are determined largely by the source of the material, the stability of the target molecule, the chromatographic techniques that will be employed, and the intended use of the product. These subjects are dealt with in general terms in the *Protein Purification Handbook* and more specifically according to target molecule in the *Recombinant Protein Handbook*, and *Antibody Purification Handbook*, available from GE Healthcare.

Sample clarification

Centrifugation and filtration are standard laboratory techniques for sample clarification and are used routinely when handling small samples.



It is highly recommended to centrifuge and filter any sample immediately before chromatographic purification.

Centrifugation

Centrifugation removes lipids and particulate matter, such as cell debris. If the sample is still not clear after centrifugation, use filter paper or a 5 μm filter as a first step and one of the filters below as a second step filter.



For small sample volumes or proteins that adsorb to filters, centrifuge at $10\,000 \times g$ for 15 min.



For cell lysates, centrifuge at $40\,000$ to $50\,000 \times g$ for 30 min.



Serum samples can be filtered through glass wool after centrifugation to remove any remaining lipids.

Filtration

Filtration removes particulate matter. Membrane filters that give the least amount of nonspecific binding of proteins are composed of cellulose acetate or PVDF.

For sample preparation before chromatography, select a filter pore size in relation to the bead size of the chromatographic medium (Table A3.1).

Table A3.1. Filter pore size recommendations

Nominal pore size of filter	Particle size of chromatography medium
1 μm	90 μm and upwards
0.45 μm	34 μm
0.22 μm	3, 10, 15 μm or when extra clean samples or sterile filtration is required



Check the recovery of the target protein in a test run. Some proteins can adsorb nonspecifically to filter surfaces.

Desalting

Detailed procedures for buffer exchange and desalting are given in Chapter 5.

Denaturation

Table A3.2. Common denaturing agents

Denaturing agent	Typical conditions for use	Removal/comment
Urea	2 to 6 M	Remove using Sephadex G-25
Guanidine hydrochloride	3 to 6 M	Remove using Sephadex G-25

Details taken from: Scopes R.K., *Protein Purification, Principles and Practice*, Springer, (1994), J.C. Janson and L. Rydén, *Protein Purification, Principles, High Resolution Methods and Applications*, 2nd ed. Wiley Inc, (1998) and other sources.

Precipitation and resolubilization

Specific sample preparation steps might be required if the crude sample is known to contain contaminants such as lipids, lipoproteins, or phenol red, which can build up on a column. Sample preparation can also be required if certain gross impurities, such as bulk protein, need be removed before any chromatographic step.

Fractional precipitation is occasionally used at laboratory scale to remove gross impurities but is generally not required in purification of affinity-tagged proteins. In some cases, precipitation can be useful as a combined protein concentration and purification step.

Precipitation techniques separate fractions by the principle of differential solubility. For example, because protein species differ in their degree of hydrophobicity, increased salt concentrations can enhance hydrophobic interactions between the proteins and cause precipitation. Fractional precipitation can be applied to remove gross impurities in three different ways, as shown in Figure A3.1.

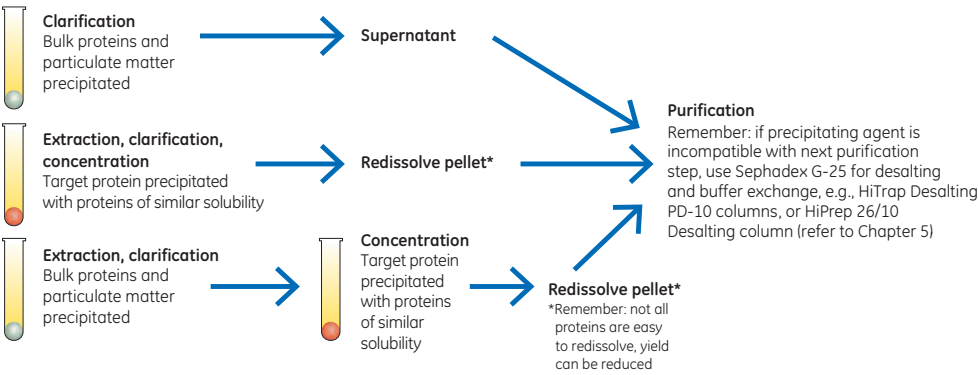


Fig A3.1. Three ways to use precipitation.

Precipitation techniques can be affected by temperature, pH, and sample concentration. These parameters must be controlled to ensure reproducible results.

Most precipitation techniques are not suitable for large-scale preparation.

Examples of precipitation agents are reviewed in Table A3.3. The most common precipitation method using ammonium sulfate is described in more detail below.

Table A3.3. Examples of precipitation techniques

Precipitation agent	Typical conditions for use	Sample type	Comment
Ammonium sulfate	As described below.	> 1 mg/ml proteins, especially immunoglobulins.	Stabilizes proteins, no denaturation; supernatant can go directly to HIC. Helps to reduce lipid content.
Dextran sulfate	Add 0.04 ml of 10% dextran sulfate and 1 ml of 1 M CaCl ₂ per ml of sample, mix 15 min, centrifuge at 10 000 × g, discard pellet.	Samples with high levels of lipoprotein, e.g., ascites.	Precipitates lipoprotein.
Polyvinylpyrrolidone	Add 3% (w/v), stir 4 h, centrifuge at 17 000 × g, discard pellet.	Samples with high levels of lipoprotein, e.g., ascites.	Alternative to dextran sulfate.
Polyethylene glycol (PEG, M _r > 4000)	Up to 20% (w/v).	Plasma proteins.	No denaturation, supernatant goes directly to IEX or AC, complete removal can be difficult. Stabilizes proteins.
Acetone (cold)	Up to 80% (v/v) at 0°C. Collect pellet after centrifugation at full speed in microcentrifuge.		Can denature protein irreversibly. Useful for peptide precipitation or concentration of sample for electrophoresis.
Polyethyleneimine	0.1% (w/v).		Precipitates aggregated nucleoproteins.
Protamine sulfate	1% (w/v).		Precipitates aggregated nucleoproteins.
Streptomycin sulfate	1% (w/v).		Precipitates nucleic acids.
Caprylic acid	(X/15) g where X = volume of sample.	Antibody concentration should be > 1 mg/ml.	Precipitates bulk of proteins from sera or ascites, leaving immunoglobulins in solution.

Details taken from: Scopes R.K., Protein Purification, Principles and Practice, Springer, (1994), J.C. Janson and L. Rydén, Protein Purification, Principles, High Resolution Methods and Applications, 2nd ed. Wiley Inc, (1998).

Ammonium sulfate precipitation

Ammonium sulfate precipitation is frequently used for initial sample concentration and clean up. As the concentration of the salt is increased, proteins will begin to “salt out.” Different proteins salt out at different concentrations, a process that can be taken advantage of to remove contaminating proteins from the crude extract. The salt concentration needs to be optimized to remove contaminants and not the desired protein. An additional step with increased salt concentration should then precipitate the target protein. If the target protein cannot be safely precipitated and redissolved, only the first step should be employed. HIC is often an excellent next purification step, as the sample already contains a high salt concentration and can be applied directly to the HIC column with little or no additional preparation. The elevated salt level enhances the interaction between the hydrophobic components of the sample and the chromatography medium.

Solutions needed for precipitation:

Saturated ammonium sulfate solution (add 100 g ammonium sulfate to 100 ml distilled water, stir to dissolve).

1 M Tris-HCl, pH 8.0.

Buffer for first purification step.



Some proteins can be damaged by ammonium sulfate. Take care when adding crystalline ammonium sulfate: high local concentrations can cause contamination of the precipitate with unwanted proteins.



For routine, reproducible purification, precipitation with ammonium sulfate should be avoided in favor of chromatography.



In general, precipitation is rarely effective for protein concentrations below 1 mg/ml.

1. Filter (0.45 μ m) or centrifuge the sample (10 000 \times g at 4°C).
2. Add 1 part 1 M Tris-HCl, pH 8.0 to 10 parts sample volume to maintain pH.
3. Stir gently. Add ammonium sulfate solution, drop by drop. Add up to 50% saturation*. Stir for 1 h.
4. Centrifuge for 20 min at 10 000 \times g.
5. Remove supernatant. Wash the pellet twice by resuspension in an equal volume of ammonium sulfate solution of the same concentration (i.e., a solution that will not redissolve the precipitated protein or cause further precipitation). Centrifuge again.
6. Dissolve the pellet in a small volume of the buffer to be used for the next step.
- 7 Ammonium sulfate is removed during clarification/buffer exchange steps with Sephadex G-25 using desalting columns (see Chapter 5).

* The percentage saturation can be adjusted either to precipitate a target molecule or to precipitate contaminants.

The quantity of ammonium sulfate required to reach a given degree of saturation varies according to temperature. Table A3.4 shows the quantities required at 20°C.

Table A3.4. Quantities of ammonium sulfate required to reach given degrees of saturation at 20°C

	Final percent saturation to be obtained																		
	20	25	30	35	40	45	50	55	60	65	70	75	80	85	90	95	100		
Starting percent	Amount of ammonium sulfate to add (grams) per liter of solution at 20°C saturation																		
0	113	144	176	208	242	277	314	351	390	430	472	516	561	608	657	708	761		
5	85	115	146	179	212	246	282	319	358	397	439	481	526	572	621	671	723		
10	57	86	117	149	182	216	251	287	325	364	405	447	491	537	584	634	685		
15	28	58	88	119	151	185	219	255	293	331	371	413	456	501	548	596	647		
20	0	29	59	89	121	154	188	223	260	298	337	378	421	465	511	559	609		
25		0	29	60	91	123	157	191	228	265	304	344	386	429	475	522	571		
30			0	30	61	92	125	160	195	232	270	309	351	393	438	485	533		
35				0	30	62	94	128	163	199	236	275	316	358	402	447	495		
40					0	31	63	96	130	166	202	241	281	322	365	410	457		
45						0	31	64	98	132	169	206	245	286	329	373	419		
50							0	32	65	99	135	172	210	250	292	335	381		
55								0	33	66	101	138	175	215	256	298	343		
60									0	33	67	103	140	179	219	261	305		
65										0	34	69	105	143	183	224	267		
70											0	34	70	107	146	186	228		
75												0	35	72	110	149	190		
80													0	36	73	112	152		
85														0	37	75	114		
90															0	37	76		
95																	0	38	

Removal of lipoproteins

Lipoproteins and other lipid material can rapidly clog chromatography columns and it is advisable to remove them before beginning purification. Precipitation agents such as dextran sulfate and polyvinylpyrrolidone, described under Fractional precipitation, are recommended to remove high levels of lipoproteins from samples such as ascites fluid.



Centrifuge samples to avoid the risk of nonspecific binding of the target molecule to a filter.



Samples such as serum can be filtered through glass wool to remove remaining lipids.

Appendix 4

Selection of purification equipment

Simple buffer exchange and desalting steps can be performed using a syringe or peristaltic pump together with prepacked HiTrap columns. A chromatography system is needed to deliver accurately controlled flow rates for high-resolution separations.

System recommendations for high-resolution SEC columns

The small bed volume of 3.2/300, and 5/150 columns makes them sensitive to dead volumes in the system. For these columns, use of systems like ÄKTA pure 25, ÄKTAmicro, or ÄKTApurifier 10 is recommended. Use short, narrow tubings and avoid unnecessary components in the flow path. Note that ÄKTA start is not compatible with the columns due to low maximum operating pressure.

The 10/300 column has a larger bed volume and can be used in systems like ÄKTA avant 25 and ÄKTAexplorer 10 in addition to the systems mentioned above. Note that ÄKTA start is not compatible with the column due to low maximum operating pressure. ÄKTA start is mainly recommended for use with HiTrap desalting columns and HiPrep Sephacryl columns. See Selection guide *Prepacked chromatography columns for ÄKTA systems*, 28-9317-78.

Note: Be aware of pressure limits.

Table A4.1. Selection of purification equipment for buffer exchange and high-resolution separations

Way of working	ÄKTA protein purification system					Syringe or peristaltic pump + HiTrap Desalting column	Gravity-fed columns
	ÄKTA start	ÄKTAprime plus	ÄKTAxpress	ÄKTA pure	ÄKTA avant		
Simple, one-step desalting, buffer exchange	x	x	x	x	x	x	x
Automated and reproducible protein purification using all common techniques including support for gradient elution	x	x	x	x	x		
Software compatible with regulatory requirements, e.g., GLP			x	x	x		
Method development and optimization using Design of Experiments (DoE)				(x)	x		
Automatic buffer preparation					x		
Automatic pH scouting				(x)	x		
Automatic media or column scouting				(x)	x		
Automatic multistep purification		(x)	x	(x)			
Scale-up, process development				(x)	x		
Software ¹ for system control and data handling	UNICORN start	PrimeView ²	UNICORN 5	UNICORN 6	UNICORN 6		

¹ A specific software version might be needed for the chosen system. See the web page for each respective system at www.gelifesciences.com

² With PrimeView, you can monitor results and evaluate data but not create methods nor control the system.

x = included

(x) = optional

DoE = Design of experiments



ÄKTA start



ÄKTAprime plus



ÄKTAexpress



ÄKTA pure



ÄKTA avant

Fig A4.1. Selection of chromatography systems from GE Healthcare suitable for size exclusion chromatography, buffer exchange, or desalting.

Appendix 5

Converting from linear flow (cm/h) to volumetric flow rates (ml/min) and *vice versa*

It is convenient when comparing results for columns of different sizes to express flow as linear flow rate (cm/h). However, flow is usually measured in volumetric flow rate (ml/min). To convert between linear flow and volumetric flow rate use one of the formulas below:

From linear flow (cm/h) to volumetric flow rate (ml/min)

$$\begin{aligned}\text{Volumetric flow rate (ml/min)} &= \frac{\text{Linear flow (cm/h)}}{60} \times \text{column cross-sectional area (cm}^2\text{)} \\ &= \frac{Y}{60} \times \frac{\pi \times d^2}{4}\end{aligned}$$

where

Y = linear flow in cm/h

d = column inner diameter in cm

Example:

What is the volumetric flow rate in an XK 16/70 column (i.d. 1.6 cm) when the linear flow is 150 cm/h?

Y = linear flow = 150 cm/h

d = inner diameter of the column = 1.6 cm

$$\begin{aligned}\text{Volumetric flow rate} &= \frac{150 \times \pi \times 1.6 \times 1.6}{60 \times 4} \text{ ml/min} \\ &= 5.03 \text{ ml/min}\end{aligned}$$

From volumetric flow rate (ml/min) to linear flow (cm/h)

$$\begin{aligned}\text{Linear flow (cm/h)} &= \frac{\text{Volumetric flow rate (ml/min)} \times 60}{\text{column cross-sectional area (cm}^2\text{)}} \\ &= Z \times 60 \times \frac{4}{\pi \times d^2}\end{aligned}$$

where

Z = volumetric flow rate in ml/min

d = column inner diameter in cm

Example:

What is the linear flow in a Tricorn 5/50 column (i.d. 0.5 cm) when the volumetric flow rate is 1 ml/min?

Z = Volumetric flow rate = 1 ml/min

d = column inner diameter = 0.5 cm

$$\begin{aligned}\text{Linear flow} &= 1 \times 60 \times \frac{4}{\pi \times 0.5 \times 0.5} \text{ cm/h} \\ &= 305.6 \text{ cm/h}\end{aligned}$$

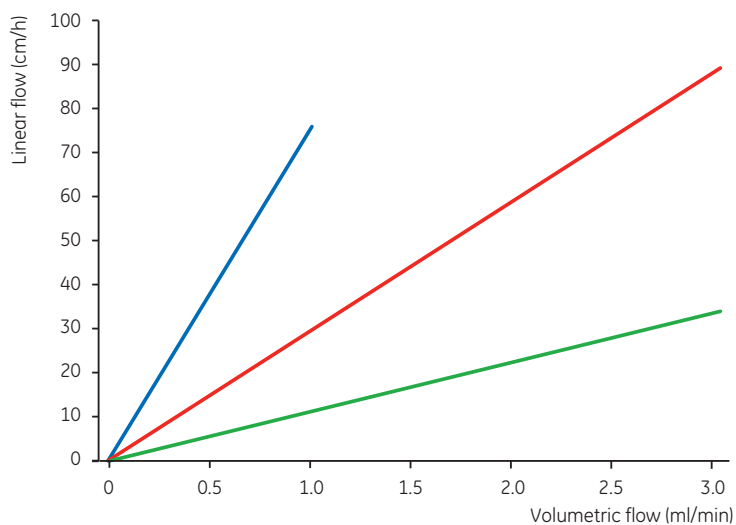


Fig A5.1. Linear flow as a function of volumetric flow: Blue curve 10 mm, red curve 16 mm, and green curve 26 mm column diameter.

From ml/min to using a syringe

1 ml/min = approximately 30 drops/min on a HiTrap 1 ml column

5 ml/min = approximately 120 drops/min on a HiTrap 5 ml column

Appendix 6

Conversion data

Proteins

Protein size and amount conversion		
Mass (g/mol)	1 µg protein	1 nmol protein
10 000	100 pmol; 6×10^{13} molecules	10 µg
50 000	20 pmol; 1.2×10^{13} molecules	50 µg
100 000	10 pmol; 6.0×10^{12} molecules	100 µg
150 000	6.7 pmol; 4.0×10^{12} molecules	150 µg

Absorbance coefficient for proteins	
Protein	A ₂₈₀ for 1 mg/ml
IgG	1.35
IgM	1.20
IgA	1.30
Protein A	0.17
Avidin	1.50
Streptavidin	3.40
Bovine serum albumin	0.70

Nucleic Acids

Approximate molecular weights (M_r) of nucleic acids

$$M_r \text{ of ssRNA} = (\# \text{ nucleotides} \times 320.5) + 159.0$$

$$M_r \text{ of ssDNA} = (\# \text{ nucleotides} \times 303.7) + 79.0$$

$$M_r \text{ of dsDNA} = (\# \text{ nucleotides} \times 607.4) + 157.9$$

Absorbance units to nucleic acid concentration conversion

$$1 A_{280} \text{ dsDNA} = 50 \mu\text{g/ml}$$

$$1 A_{280} \text{ ssDNA} = 37 \mu\text{g/ml}$$

$$1 A_{280} \text{ ssRNA} = 40 \mu\text{g/ml}$$

Column pressures

The maximum operating back pressure refers to the pressure above which the column contents can begin to compress.

Pressure units may be expressed in megaPascal (MPa), bar, or pounds per square inch (psi) and can be converted as follows: 1 MPa = 10 bar = 145 psi.

Appendix 7

Amino acids table

Amino acid	Three-letter code	Single-letter code	Structure
Alanine	Ala	A	
Arginine	Arg	R	
Asparagine	Asn	N	
Aspartic Acid	Asp	D	
Cysteine	Cys	C	
Glutamic Acid	Glu	E	
Glutamine	Gln	Q	
Glycine	Gly	G	
Histidine	His	H	
Isoleucine	Ile	I	
Leucine	Leu	L	
Lysine	Lys	K	
Methionine	Met	M	
Phenylalanine	Phe	F	
Proline	Pro	P	
Serine	Ser	S	
Threonine	Thr	T	
Tryptophan	Trp	W	
Tyrosine	Tyr	Y	
Valine	Val	V	

Formula	M _r	Middle unit residue (-H ₂ O)		Side-chain charge at neutral pH	Hydrophilic (nonpolar)	Uncharged (polar)	Hydrophilic (polar)
		Formula	M _r				
C ₃ H ₇ NO ₂	89.1	C ₃ H ₅ NO	71.1	Neutral	●		
C ₆ H ₁₄ N ₄ O ₂	174.2	C ₆ H ₁₂ N ₄ O	156.2	Basic (+ve)			●
C ₄ H ₈ N ₂ O ₃	132.1	C ₄ H ₆ N ₂ O	114.1	Neutral		●	
C ₄ H ₇ NO ₄	133.1	C ₄ H ₅ NO ₃	115.1	Acidic (+ve)			●
C ₃ H ₇ NO ₂ S	121.2	C ₃ H ₅ NOS	103.2	Neutral		●	
C ₅ H ₉ NO ₄	147.1	C ₅ H ₇ NO ₃	129.1	Acidic (+ve)			●
C ₅ H ₁₀ N ₂ O ₃	146.1	C ₅ H ₈ N ₂ O ₂	128.1	Neutral		●	
C ₂ H ₅ NO ₂	75.1	C ₂ H ₃ NO	57.1	Neutral		●	
C ₆ H ₉ N ₃ O ₂	155.2	C ₆ H ₇ N ₃ O	137.2	Basic (+ve)			●
C ₆ H ₁₃ NO ₂	131.2	C ₆ H ₁₁ NO	113.2	Neutral	●		
C ₆ H ₁₃ NO ₂	131.2	C ₆ H ₁₁ NO	113.2	Neutral	●		
C ₆ H ₁₄ N ₂ O ₂	146.2	C ₆ H ₁₂ N ₂ O	128.2	Basic (+ve)			●
C ₅ H ₁₁ NO ₂ S	149.2	C ₅ H ₉ NOS	131.2	Neutral	●		
C ₉ H ₁₁ NO ₂	165.2	C ₉ H ₉ NO	147.2	Neutral	●		
C ₅ H ₉ NO ₂	115.1	C ₅ H ₇ NO	97.1	Neutral	●		
C ₃ H ₇ NO ₃	105.1	C ₃ H ₅ NO ₂	87.1	Neutral		●	
C ₄ H ₉ NO ₃	119.1	C ₄ H ₇ NO ₂	101.1	Neutral		●	
C ₁₁ H ₁₂ N ₂ O ₂	204.2	C ₁₁ H ₁₀ N ₂ O	186.2	Neutral	●		
C ₉ H ₁₁ NO ₃	181.2	C ₉ H ₉ NO ₂	163.2	Neutral		●	
C ₅ H ₁₁ NO ₂	117.1	C ₅ H ₉ NO	99.1	Neutral	●		

Appendix 8

Analysis and characterization

Analytical assays are essential to follow the progress of purification. They are used to assess the effectiveness of the purification in terms of yield, biological activity, recovery, and degree of purification. The importance of a reliable assay for the target molecule cannot be overemphasized.

Protein detection and quantitation

Detection and quantitation of the target protein are needed when optimizing purification protocols. For overexpressed proteins, the high concentration in itself can be used for detection of the target protein fraction in a chromatogram, but in such a case verification of the identity of the protein in the final preparation is needed. Specific detection of tagged proteins can often be accomplished by analyzing the presence of the tag by activity or immunoassay, or simply by the spectral properties of the tag. Specific detection of the target protein can be obtained by functional assays, immunodetection, and mass spectrometry. SDS-polyacrylamide gel electrophoresis (SDS-PAGE) is the key method for checking purity of proteins. The target protein band can often be identified using the apparent molecular weight obtained by including standard molecular weight markers in the analysis. Subsequent verification of protein identity should always be obtained. Optimizing purification protocols can require functional assays to assess the intactness of the target protein. In general:

- The relative yield of tagged protein can often be determined by measuring the absorbance at 280 nm because the purity after a single purification step is high, that is, most of the eluted material may be considered to be the target protein. The extinction coefficient of the target protein will be needed. A good estimation can be obtained by theoretical calculation from the amino acid composition of the protein.
- The yield of protein may also be determined by standard chromogenic methods (e.g., Lowry, BCA™ protein assay, and Bradford total protein assay).
- Immunoassays (Western blot, ELISA, and immunoprecipitation) can be used for quantitation if a suitable standard curve can be produced. In this case, it is not necessary to purify the tagged protein so long as a purified standard is available. Therefore, these techniques may be used for quantitation during protocol development. The immunoassay technique is also particularly suitable for screening large numbers of samples when a simple yes/no answer is required (e.g., when testing fractions from a chromatographic run).

Purity check and protein characterization

Purity

Purity of the target protein is most often estimated by SDS-PAGE, capillary electrophoresis, RPC, or mass spectrometry. The absorbance at 280 nm gives a rough but fast and nondestructive estimate of total protein content in crude samples. Lowry or Bradford assays are also frequently used to determine the total protein. The Bradford assay is particularly suited to samples where there is a high lipid content that can interfere with the Lowry assay. Absorbance data can be calibrated to high accuracy for pure proteins.

Obtaining a single band in electrophoresis is indicative of a pure protein, although potentially other proteins can comigrate. At this stage, additional methods based on orthogonal separation principles, such as chromatography in analytical scale should be used to confirm homogeneity/purity.

Characterization

Characterization of purified components can be divided into physical, chemical, and biological/functional characterization.

Physical parameters

Physical parameters important for identification, further experimental work, and documentation include mass, isoelectric point, and UV/Vis spectral properties.

Mass is conveniently determined with mass spectrometry (MS) for proteins, with accuracy greater than 0.1%, providing a good fingerprint. Differences in single amino acids or attached monosaccharides are clearly revealed.

Isoelectric point (pI) is determined by analytical isoelectric focusing (IEF) with accuracy greater than 0.1 pH units. IEF can sometimes reveal variations among noncharged amino acids in the vicinity of charged ones.

The UV/Vis spectrum can sometimes be unique for a specific protein, in particular if light-absorbing cofactors (flavins, heme groups, or other metal ions) are present. The specific extinction coefficient can also be calibrated, allowing very accurate concentration determination once the protein is free from contaminants.

Chemical characterization

Chemical characterization includes total amino acid composition, complete or partial amino acid sequence, MS fragment pattern (peptide maps) and determination of post-translational modifications including glycosylation. The total amino acid composition is still carried out in specialized laboratories, while most other data can be obtained by different applications of MS.

Functional characterization

Biological/functional characterization comprises enzymatic specificity and kinetic parameters including the action of inhibitors. Examples of important nonenzymatic properties are binding to signal substances, toxins, lectins, and antibodies. The interaction of a component with detecting antibodies can also be found in this category.

Enzymatic properties are determined by a multitude of specific protocols. Readily reversible protein-ligand interactions are typically determined by electrophoretic or chromatographic methods, whereas slow (strong) protein-ligand interactions are determined by filter-binding assays. Protein-protein interactions and many protein-ligand interactions can be conveniently studied with Biacore™ label-free interaction assays that also allow the study of binding kinetics.







	Sensitivity limit	Quantitative	Living cells	Linear dynamic range
Coomassie blue staining	20 ng	+++	no	7
Negative staining	15 ng	+	no	3
Silver staining	200 pg	++	no	3
Fluorescent staining	400 pg	++++	no	10 ⁴
Fluorescent labeling	a few picogram	+++++	no	10 ⁶
<i>Radioactive labeling:</i>				
X-ray film	1 pg	+++	yes	20
Phosphor-imager plates	0.2 pg	++++	yes	10 ⁵
Stable-isotope labeling	< 1 pg	++++ (with MS)	yes	N/A

Appendix 9








Storage of biological samples

The advice given here is of a general nature and cannot be applied to every biological sample. Always consider the properties of the specific sample and its intended use before following any of these recommendations.

General recommendations

-  Add stabilizing agents when necessary. Stabilizing agents are often required for storage of purified proteins.
-  Serum, culture supernatants, and ascites should be kept frozen at -20°C or -70°C, in small aliquots.
-  Avoid repeated freeze/thawing or freeze drying/redissolving that can reduce biological activity.
-  Avoid conditions close to stability limits, in terms of for example pH or salt concentrations, reducing, or chelating agents.
-  Keep refrigerated at 4°C in a closed vessel to minimize bacterial growth and protease activity. For prolonged storage at 4°C (more than 24 h), add a preserving agent (e.g., merthiolate 0.01%).
-  Sodium azide can interfere with coupling methods, and some biological assays, and can be a health hazard. It can be removed by using a desalting column (see Chapter 5).

Common storage conditions for purified proteins

-  Store as a precipitate in a high concentration of, for example, 4 M ammonium sulfate.
-  Freeze in 50% glycerol, especially suitable for enzymes.
-  Avoid using preserving agents if the product is to be used for a biological assay. Preserving agents should not be added if *in vivo* experiments are to be performed. Store samples in small aliquots and keep frozen.
-  Sterile filter to prolong storage time.
-  Add stabilizing agents, for example, glycerol (5% to 20%), serum albumin (10 mg/ml), ligand (concentration is selected based on concentration of active protein) to maintain biological activity. Remember that any additive will reduce the purity of the protein and might need to be removed at a later stage.
-  Avoid repeated freeze/thawing or freeze drying/redissolving that can reduce biological activity.
-  Certain proteins, including some mouse antibodies of the IgG₃ subclass, should not be stored at 4°C as they precipitate at this temperature (cryoproteins). Store at room temperature in the presence of a preserving agent.

Appendix 10

Molecular weight estimation and molecular weight distribution analysis

Unlike electrophoretic techniques, SEC provides a means of determining the molecular weight or size (Stokes radius) of native or denatured proteins under a wide variety of conditions of pH, ionic strength and temperature, free from the constraints imposed by the charge state of the molecules. In order to understand and follow the procedures outlined, it is important to have read Chapter 7, SEC in theory.

For molecular weight determination, several theoretical models have been proposed to describe the behavior of solutes during SEC. Most models assume that the partition of solute molecules between the particles and surrounding liquid is an entirely steric effect. However, in practice a homologous series of compounds demonstrate a sigmoidal relationship between their various elution volume parameters and the logarithm of their molecular weights. Thus, molecular weight determination by SEC can be made by comparing an elution volume parameter, such as K_{av} of the substance of interest, with the values obtained for several known calibration standards.

A calibration curve is prepared by measuring the elution volumes of several standards, calculating their corresponding K_{av} values (or similar parameter), and plotting their K_{av} values versus the logarithm of their molecular weight. The molecular weight of an unknown substance can be determined from the calibration curve once its K_{av} value is calculated from its measured elution volume. Various elution parameters, such as V_e , V_e/V_o , K_d , and K_{av} have been used in the literature for the preparation of calibration curves but the use of K_{av} is recommended since: 1) it is less sensitive to errors which can be introduced as a result of variations in column preparation and column dimensions, 2) it does not require the unreliable determination of the internal volume (V_i) as is required with K_d .

For good estimation of molecular weight, the calibration standards must have the same relationship between molecular weight and molecular size as the substance of interest. Calibration Kits from GE Healthcare provide well-characterized, globular protein standards for protein molecular weight estimation. The Low Molecular Weight (LMW) Gel Filtration Calibration Kit contains five individually lyophilized proteins with molecular weights in the range 6500 to 75 000 and Blue Dextran 2000 (Table A10.1). The High Molecular Weight (HMW) Gel Filtration Calibration Kit contains five individually lyophilized proteins with molecular weights in the range 43 000 to 669 000 and Blue Dextran 2000 (Table A10.2). Blue Dextran 2000 determines the void fraction in the column.

These well-defined protein standards show excellent behavior in SEC and enable simple, reliable calibration of SEC columns.

Table A10.1. Characteristics of Gel Filtration Calibration Kit LMW

Protein (weight per vial)	Molecular weight (M_r)	Source
Aprotinin (10 mg)	6500	Bovine lung
Ribonuclease A (50 mg)	13 700	Bovine pancreas
Carbonic anhydrase (15 mg)	29 000	Bovine erythrocytes
Ovalbumin (50 mg)	43 000	Hen egg
Conalbumin (50 mg)	75 000	Chicken egg white
Blue Dextran 2000 (50 mg)	2 000 000	

Table A10.2. Characteristics of Gel Filtration Calibration HMW

Protein (weight per vial)	Molecular weight (M _r)	Source
Ovalbumin (50 mg)	43 000	Hen egg
Conalbumin (50 mg)	75 000	Chicken egg white
Aldolase ¹ (50 mg)	158 000	Rabbit muscle
Ferritin ¹ (15 mg)	440 000	Horse spleen
Thyroglobulin (50 mg)	669 000	Bovine thyroid
Blue Dextran 2000 (50 mg)	2 000 000	

¹ These proteins are supplied mixed with sucrose or mannitol to maintain stability and aid their solubility.

Typical calibration results from chromatographic runs and calculated calibration curves using prepacked Superdex columns are shown in Figures A10.1 and A10.2.

The method used for Figures A10.1 and A10.2:

Sample: Proteins from Gel Filtration Calibration Kits LMW and HMW: aprotinin (Apr), RNase A (R), carbonic anhydrase (CA), ovalbumin (O), conalbumin (C), aldolase (Ald), ferritin (F), and thyroglobulin (T)

Sample vol.: Figures A10.1 and A10.2, 100 µl

Buffer: 50 mM phosphate buffer, 150 mM sodium chloride, pH 7.2

Flow rate: Figure A10.1, 0.5 ml/min
Figure A10.2, 0.6 ml/min

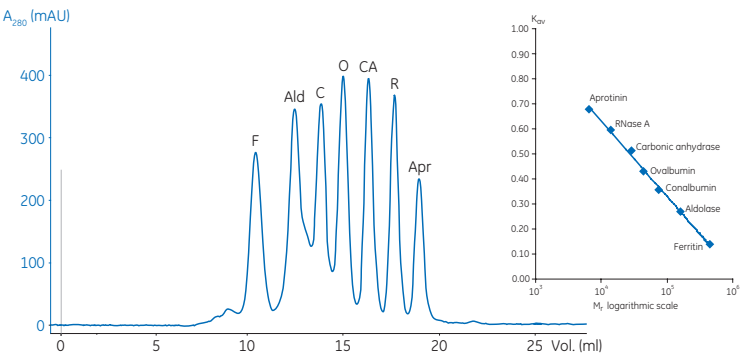


Fig A10.1. Chromatographic separation and calibration curve for the standard proteins on Superdex 200 10/300 GL column.

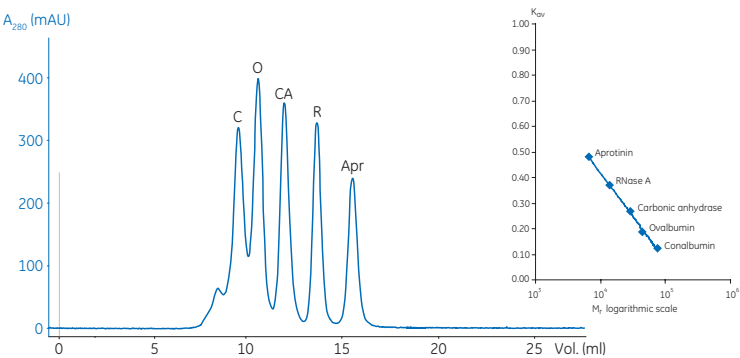


Fig A10.2. Chromatographic separation and calibration curve for the standard proteins on Superdex 75 10/300 GL column.

Many of the parameters important for a successful molecular weight determination are the same as for any high-resolution fractionation:



Use a medium with the correct fractionation range for the molecules of interest. The expected molecular weight values should fall in the linear part of the selectivity curve (see SEC media fractionation guide, Chapter 1).



Use a prepacked column whenever possible. Homemade columns must be packed very carefully (see Appendix 1).



Use freshly prepared calibration standards, selected so that the expected molecular weight values are covered by the entire calibration range. Always filter Blue Dextran 2000 before use. Apply samples in a volume less than 2% of the total column volume.



Use the same buffer for the separation of calibrants and sample, for example 50 mM sodium phosphate, 150 mM sodium chloride at pH 7. Use the recommended flow rate for the prepacked column or medium selected.



If the molecular weight is unknown, use a medium with a wide fractionation range such as Sephacryl HR. This is also recommended for molecular weight distribution analysis and for polymeric materials such as dextrans and polyethylene glycols.



Performing a molecular weight determination in the presence of urea, guanidine hydrochloride, or SDS transforms polypeptides and proteins to a random coil configuration and so reduces structural differences. Differences will be seen in the resulting molecular weight values when compared to values acquired under nondenaturing conditions.

Deviation from a K_{av} :log M_r calibration curve can occur if the molecule of interest does not have the same molecular shape as the standards.

Performing a molecular weight determination

1. If using a self-packed column, prepare a fresh, filtered solution of Blue Dextran 2000 (1 mg/ml) in the running buffer. Apply Blue Dextran to the column, using a volume < 2% of the total column volume (V_t) to determine the void volume (V_o), and to check the column packing.
2. Dissolve the selected calibration references in the running buffer (at concentrations recommended by the manufacturer). Allow a few minutes for dissolution, stirring gently. Do not heat or mix vigorously. If necessary, filter the calibration solution.
3. Apply the calibration solution to the column, in a volume < 2% of the total column volume (V_t).
4. Determine the elution volumes (V_e) for the standards by measuring the volume of the eluent from the point of application to the centre of the elution peak.
5. Calculate the K_{av} values for the standards and prepare a calibration curve of K_{av} versus the logarithm of their molecular weights, as follows:

$$K_{av} = \frac{V_e - V_o}{V_t - V_o}$$

where V_e = elution volume for the protein

V_o = column void volume = elution volume for Blue Dextran 2000

V_t = total bed volume

Use a computer to plot the K_{av} value for each protein standard against the corresponding logarithmic molecular weight and use Microsoft® Excel® to calculate the regression line.

6. Apply the sample in a volume $< 2\%$ of the total column volume (V_t) and determine the elution volume (V_e) of the molecule of interest.
7. Calculate the corresponding K_{av} for the component of interest and determine its molecular weight from the calibration curve.



A calibrated column can be used for extended periods as long as the column is kept in good condition and not allowed to dry out, eliminating the need to set up a separate experiment for each determination.

Product index

ÄKTA avant chromatography system	112–113	Sephacryl S-300 HR	23, 59, 62 , 65, 102
ÄKTAexplorer chromatography system	53, 112	Sephacryl S-400 HR	23, 59, 61–62 , 65, 102
ÄKTAmicro chromatography system	19, 22, 47, 52, 55, 112	Sephacryl S-500 HR	23, 59, 62 , 65, 102
ÄKTAprime chromatography system	72	Sephacryl S-1000 SF	23, 59, 62 , 65
ÄKTAprime plus chromatography system	76, 113	Sephadex G-10	16, 23–24, 67–69 , 77, 80, 83, 103, 105–106
ÄKTApurifier chromatography system	30, 40, 112	Sephadex G-25 Superfine	23–24, 67 , 69–70, 74, 80, 103, 106
ÄKTA start chromatography system	112–113	Sephadex G-25 Fine	23, 67 , 69–70, 80, 103, 106
ÄKTAxpress chromatography system	112–113	Sephadex G-25 Medium	67 , 69–70, 80, 103, 106
Blue Dextran 2000	61, 123, 124, 125	Sephadex G-25 Coarse	23, 34, 67, 80, 103, 106
Gel Filtration Calibration Kit LMW	123–124	Sephadex LH-20	83–87
Gel Filtration Calibration Kit HMW	123–124	Solvent resistant (SR) empty columns	85, 88
HiLoad 16/600 Superdex 30 prep grade	31	Superdex 75 3.2/300	45
HiLoad 16/600 Superdex 75 prep grade	44	Superdex 75 5/150 GL	18, 45, 48
HiLoad 16/600 Superdex 200 prep grade	20, 44	Superdex 75 10/300 GL	43 , 45, 124
HiPrep 26/10 Desalting	67–69, 71–74 , 76, 78–79, 81, 108	Superdex 200 Increase 3.2/300	30 , 45
HiPrep 16/60 Sephacryl S-100 HR	60 , 62	Superdex 200 Increase 5/150 GL	18–19 , 45–47, 49
HiPrep 26/60 Sephacryl S-100 HR	62–63	Superdex 200 Increase 10/300 GL	22, 40, 45–46
HiPrep 16/60 Sephacryl S-200 HR	60 , 62	Superdex 200 3.2/300	45
HiPrep 26/60 Sephacryl S-200 HR	62	Superdex 200 10/300 GL	40 , 45, 124
HiPrep 16/60 Sephacryl S-300 HR	60 , 62	Superdex Peptide 3.2/300	45
HiPrep 26/60 Sephacryl S-300 HR	62	Superdex Peptide 10/300 GL	42, 45,
HiPrep 16/60 Sephacryl S-400 HR	60 , 62	Superdex 30 prep grade	23, 31, 39, 43, 44 , 45, 46, 50, 92
HiPrep 26/60 Sephacryl S-400 HR	62	Superdex 75 prep grade	23, 39, 43, 44 , 45, 50, 92, 97
HiPrep 16/60 Sephacryl S-500 HR	60 , 62	Superdex 200 prep grade	20, 23, 25, 39, 43–44, 45, 50, 92
HiPrep 26/60 Sephacryl S-500 HR	62	Superose 6 Increase 3.2/300	54
HiScale empty columns	100	Superose 6 Increase 5/150 GL	18, 54–55
HiTrap Chelating HP	17, 72	Superose 6 Increase 10/300 GL	22, 29, 52–53, 54
HiTrap Desalting Column	32, 67, 69, 71–79 , 81, 108, 112	Superose 6 3.2/300	54
MabSelect	97, 98	Superose 6 10/300 GL	52 , 54
MidiSpin Adapter	71	Superose 12 3.2/300	54, 55
MiniSpin Adapter	71	Superose 12 10/300 GL	54
Packing Connectors	102	Superose 6 prep grade	23, 51, 54, 57,
PD-10 Desalting Column	69, 77–78	Superose 12 prep grade	23, 53–54, 57,
PD-10 Spin Adapter	71	Tricorn columns	18, 53, 100, 114
PD MidiTrap G-25	69, 71, 73	UNICORN control software	29, 112
PD MiniTrap G-10	69, 71, 73	XK empty columns	25, 43, 61, 97, 98, 99, 100–103, 110, 114
PD MiniTrap G-25	69, 71, 73		
PD MultiTrap G-25	69, 71, 73		
PD SpinTrap G-25	69, 71, 73		
PrimeView software	112		
Sephacryl S-100 HR	23, 59, 61–62 , 65, 102		
Sephacryl S-200 HR	23, 59, 61–62 , 65, 102		

Related literature

Purification	Code number
Antibody Purification Handbook	18-1037-46
Strategies for Protein Purification Handbook	28-9833-31
Recombinant Protein Handbook, Principles and Methods	18-1142-75
Purifying Challenging Proteins, Principles and Methods	28-9095-31
Affinity Chromatography Handbook, Principles and Methods	18-1022-29
Ion Exchange Chromatography Handbook, Principles and Methods	18-1114-21
Hydrophobic Interaction and Reversed Phase Chromatography Handbook, Principles and Methods	11-0012-69
Sample preparation for analysis of proteins, peptides, and carbohydrates, Selection guide	18-1128-62
Gel filtration columns and media, Selection guide and product profile	18-1124-19
Solutions for antibody purification, Selection guide	28-9351-97
Ion exchange columns and media, Selection guide	18-1127-31
Affinity chromatography columns and media, Selection guide	18-1121-86
HiTrap - convenient protein purification, Column guide	18-1129-81
ÄKTA - protein purification by design, Brochure	28-4026-97
Prepacked chromatography columns for ÄKTA systems, Selection guide	28-9317-78
Column Packing - The Movie, CD	18-1165-33
Pure simplicity for tagged proteins, Brochure	28-9353-64
Years of experience in every column, Brochure	28-9090-94
Protein Analysis	
www.gelifesciences.com/proteinanalysis_techsupport	

Ordering information

High-resolution SEC

Column	Quantity	Code number
Superdex 200 Increase		
Superdex 200 Increase 3.2/300	1 × 2.4 ml column	28-9909-46
Superdex 200 Increase 5/150 GL	1 × 3 ml column	28-9909-45
Superdex 200 Increase 10/300 GL	1 × 24 ml column	28-9909-44
Superdex		
Superdex Peptide 3.2/300	1 × 2.4 ml column	29-0362-31
Superdex Peptide 10/300 GL	1 × 24 ml column	17-5176-01
Superdex 75 3.2/300	1 × 2.4 ml column	29-0362-30
Superdex 75 5/150 GL	1 × 3 ml column	28-9205-04
Superdex 75 10/300 GL	1 × 24 ml column	17-5174-01
Superdex 200 3.2/300*	1 × 2.4 ml column	29-0362-32
Superdex 200 5/150 GL*	1 × 3 ml column	28-9065-61
Superdex 200 10/300 GL*	1 × 24 ml column	17-5175-01
HiLoad 16/600 Superdex 30 prep grade	1 × 120 ml column	28-9893-31
HiLoad 26/600 Superdex 30 prep grade	1 × 320 ml column	28-9893-32
HiLoad 16/600 Superdex 75 prep grade	1 × 120 ml column	28-9893-33
HiLoad 26/600 Superdex 75 prep grade	1 × 320 ml column	28-9893-34
HiLoad 16/600 Superdex 200 prep grade	1 × 120 ml column	28-9893-35
HiLoad 26/600 Superdex 200 prep grade	1 × 320 ml column	28-9893-36
Superdex 30 prep grade	150 ml	17-0905-01
Superdex 75 prep grade	150 ml	17-1044-01
Superdex 200 prep grade	150 ml	17-1043-01
Superose 6 Increase		
Superose 6 Increase 3.2/300	1 × 2.4 ml column	29-0915-98
Superose 6 Increase 5/150 GL	1 × 3 ml column	29-0915-97
Superose 6 Increase 10/300 GL	1 × 24 ml column	29-0915-96
Superose		
Superose 6 3.2/300†	1 × 2.4 ml column	29-0362-26
Superose 6 10/300 GL†	1 × 24 ml column	17-5172-01
Superose 12 3.2/300	1 × 2.4 ml column	29-0362-25
Superose 12 10/300 GL	1 × 24 ml column	17-5173-01
Superose 6 prep grade	125 ml	17-0489-01
Superose 12 prep grade	125 ml	17-0536-01

* Superdex 200 3.2/300, 5/150 GL, and 10/300 GL columns are being replaced by Superdex 200 Increase columns. Superdex 200 columns will be available until December 31 2015.

† Superose 6 3.2/300 and 10/300 GL columns are to be replaced by Superose 6 Increase columns. Superose 6 columns will be available until December 31 2016.

Column	Quantity	Code number
Sephacryl		
HiPrep 16/60 Sephacryl S-100 HR	1 × 120 ml column	17-1165-01
HiPrep 26/60 Sephacryl S-100 HR	1 × 320 ml column	17-1194-01
HiPrep 16/60 Sephacryl S-200 HR	1 × 120 ml column	17-1166-01
HiPrep 26/60 Sephacryl S-200 HR	1 × 320 ml column	17-1195-01
HiPrep 16/60 Sephacryl S-300 HR	1 × 120 ml column	17-1167-01
HiPrep 26/60 Sephacryl S-300 HR	1 × 320 ml column	17-1196-01
HiPrep 16/60 Sephacryl S-400 HR	1 × 120 ml column	28-9356-04
HiPrep 26/60 Sephacryl S-400 HR	1 × 320 ml column	28-9356-05
HiPrep 16/60 Sephacryl S-500 HR	1 × 120 ml column	28-9356-06
HiPrep 26/60 Sephacryl S-500 HR	1 × 320 ml column	28-9356-07
Sephacryl S-100 HR	150 ml	17-0612-10
Sephacryl S-100 HR	750 ml	17-0612-01
Sephacryl S-200 HR	150 ml	17-0584-10
Sephacryl S-200 HR	750 ml	17-0584-01
Sephacryl S-300 HR	150 ml	17-0599-10
Sephacryl S-300 HR	750 ml	17-0599-01
Sephacryl S-400 HR	150 ml	17-0609-10
Sephacryl S-400 HR	750 ml	17-0609-01
Sephacryl S-500 HR	150 ml	17-0613-10
Sephacryl S-500 HR	750 ml	17-0613-01
Sephacryl S-1000 SF	750 ml	17-0476-01

Desalting and group separations

HiTrap Desalting	1 × 5 ml column	29-0486-84
HiTrap Desalting	5 × 5 ml columns	17-1408-01
HiPrep 26/10 Desalting	1 × 53 ml column	17-5087-01
HiPrep 26/10 Desalting	4 × 53 ml column	17-5087-02
PD-10 Desalting Column	30 gravity-fed columns	17-0851-01
Empty PD-10 Desalting Column	50 gravity-fed empty columns	17-0435-01
PD MiniTrap G-10	50 columns	28-9180-10
PD Spin Trap G-25	50 columns	28-9180-04
PD MultiTrap G-25	4 × 96-well plates	28-9180-06
PD MiniTrap G-25	50 columns	28-9180-07
PD MidiTrap G-25	50 columns	28-9180-08
MiniSpin Adapter	10	28-9232-43
MidiSpin Adapter	10	28-9232-44
PD-10 Spin Adapter	10	28-9232-45
Collection plate 500 µl V-bottom	5 × 96-well plates	28-4039-43
LabMate PD-10 Buffer Reservoir	10	18-3216-03

Column	Quantity	Code number
Sephadex G-10	100 g	17-0010-01
Sephadex G-10	500 g	17-0010-02
Sephadex G-25 Coarse	100 g	17-0034-01
Sephadex G-25 Coarse	500 g	17-0034-02
Sephadex G-25 Fine	100 g	17-0032-01
Sephadex G-25 Fine	500 g	17-0032-02
Sephadex G-25 Medium	100 g	17-0033-01
Sephadex G-25 Medium	500 g	17-0033-02
Sephadex G-25 Superfine	100 g	17-0031-01
Sephadex G-50 Fine	100 g	17-0042-01
Sephadex G-50 Fine	500 g	17-0042-02
Separation in organic solvents		
Sephadex LH-20	25 g	17-0090-10
Sephadex LH-20	100 g	17-0090-01
Sephadex LH-20	500 g	17-0090-02
Calibration Kits		
Gel Filtration Calibration Kit LMW	1	28-4038-41
Gel Filtration Calibration Kit HMW	1	28-4038-42

Empty columns

XK columns

XK 16/20 column	1	18-8773-01
XK 16/40 column	1	18-8774-01
XK 16/70 column	1	18-8775-01
XK 16/100 column	1	18-8776-01
XK 26/20 column	1	18-1000-72
XK 26/40 column	1	18-8768-01
XK 26/70 column	1	18-8769-01
XK 26/100 column	1	18-8770-01
XK 50/20 column	1	18-1000-71
XK 50/30 column	1	18-8751-01
XK 50/60 column	1	18-8752-01
XK 50/100 column	1	18-8753-01

Tricorn columns

Tricorn 10/100	1	28-4065-15
Tricorn 10/150	1	28-4064-16
Tricorn 10/200	1	28-4064-17
Tricorn 10/300	1	28-4064-18
Tricorn 10/600	1	28-4064-19

Column	Quantity	Code number
HiScale columns		
HiScale 16/20	1	28-9644-41
HiScale 16/40	1	28-9644-24
HiScale 26/20	1	28-9645-14
HiScale 26/40	1	28-9645-13
HiScale 50/20	1	28-9644-45
HiScale 50/40	1	28-9644-44
Solvent resistant columns		
SR 25/45 column	1	19-0879-01
SR 25/100 column	1	19-0880-01

Accessories and spare parts

Packing Connector XK 16	1	18-1153-44
Packing Connector XK 26	1	18-1153-45
Packing equipment 10/100 (Tricorn)	1	18-1153-25
Packing Connector 10-10	1	18-1153-23

More details and products can be found on www.gelifesciences.com/protein-purification

For local office contact information,
please visit www.gelifesciences.com/contact

www.gelifesciences.com/sizeexclusion

GE Healthcare Bio-Sciences AB
Björkgatan 30
751 84 Uppsala
Sweden



GE and GE monogram are trademarks of General Electric Company.

ÅKTA, Biacore, BioProcess, HiLoad, HiPrep, HiScale, HiTrap, MabSelect, MidiTrap, MiniTrap, MultiTrap, Sephacryl, Sephadex, Sepharose, SpinTrap, Superdex, Superose, Tricorn, and UNICORN are trademarks of GE Healthcare Company or one of its subsidiaries.

BCA is a trademark of Thermo Fisher Scientific LLC. Coomassie is a trademark of Imperial Chemical Industries Limited. Microsoft and Excel are registered trademarks of the Microsoft Corporation. Triton is a trademark of Union Carbide Chemicals and Plastic Company Inc. Tween is a trademark of Uniqema Americas LLC.

All other third-party trademarks are the property of their respective owners.

IMAC Sepharose products, Ni Sepharose products and Fe Sepharose products:
These products are sold under a license from Sigma-Aldrich under patent number EP 1276716 (Metal chelating compositions) and equivalent patents and patent applications in other countries.

© 2000–2014 General Electric Company—All rights reserved.
First published Dec. 2000.

All goods and services are sold subject to the terms and conditions of sale of the company within GE Healthcare which supplies them. A copy of these terms and conditions is available on request. Contact your local GE Healthcare representative for the most current information.

GE Healthcare UK Limited Amersham Place
Little Chalfont
Buckinghamshire, HP7 9NA
UK

GE Healthcare Europe, GmbH
Munzinger Strasse 5
D-79111 Freiburg
Germany

GE Healthcare Bio-Sciences Corp.
800 Centennial Avenue, P.O. Box 1327
Piscataway, NJ 08855-1327
USA

GE Healthcare Bio-Sciences KK
Sanken Bldg., 3-25-1, Hyakunincho
Shinjuku-ku, Tokyo 169-0073
Japan