

Vivapure Metal Chelate Mini spin columns

Technical data and operating instructions.
For *in vitro* use only.

Vivapure Metal Chelate Mini spin columns - for the purification of proteins with poly-histidine tags

Storage conditions

Vivapure Metal Chelate Mini spin columns can be stored at room temperature. They have a guaranteed shelf life of 12 months from the date of purchase.

Introduction

Vivapure Metal Chelate Mini spin columns represent a new generation of Immobilized Metal Affinity Chromatography (IMAC) purification devices, which simply can be used in a centrifuge. IMAC is a common and effective tool for the purification of poly-histidine tagged proteins. The method is based on the ability of some proteins to bind to immobilized metal ions. Especially strong interactions take place with the commonly used poly-histidine (His)₆ tag with six consecutive histidine residues. Using the IMAC principle, poly-histidine tagged proteins can be concentrated to a high degree of purity even from cell lysates or culture supernatants.

The Vivapure Metal Chelate Mini spin columns have covalently bound IDA (iminodiacetic acid) groups on the membrane. The IDA groups can be loaded with different metal ions depending on the particular application. We suggest using nickel (Ni²⁺), cobalt (Co²⁺), copper (Cu²⁺) or zinc (Zn²⁺) ions, but also different metal ions can easily be immobilized on the membrane. Proteins engineered with poly-histidine tags passing through the prepared membrane are preferentially bound. These bound proteins can be easily eluted from the membrane using buffers with varying concentrations of imidazole.

Vivapure Metal Chelate Mini spin columns are designed to simplify the chromatographic steps normally associated with IMAC. They are ideally suited for the quick and convenient purification of small amounts of poly-histidine tagged proteins (approx. 400 µg). This makes them also a convenient and quick tool for screening purposes.



Technical assistance

For more information, please contact the Vivascience Support Center.

Europe:

Tel +49 180 2000 581 (toll free)

Fax +49 180 2000 583

info@sc.vivascience.de

USA:

Tel +1 877 452 2345 (toll free)

Fax +1 760 918 8281

info.usa@vivascience.com

Vivapure Metal Chelate Mini spin columns

Cat. No.	VS-MC01MC12
Vivapure Metal Chelate Mini spin columns "m"	12
Clarification Mini spin columns	12
Collection tubes	36
Instruction Manual	1

Specifications

Max. volume per centrifuge run	400 µl
Recommended centrifugation speed	1500 x g - 2000 x g (please refer to protocol)
Binding capacity	up to 400 µg


Materials of construction

Vivapure Metal Chelate Mini spin columns	Polypropylene
Clarification Mini spin columns	Polypropylene
Collection tubes	Polypropylene

Handling overview

There are a number of various expression systems for poly-histidine tagged proteins available.

This protocol addresses protein purification from bacterial expression systems. The procedure may be adapted to other related expression systems, e.g. yeast or eukaryotic cells.

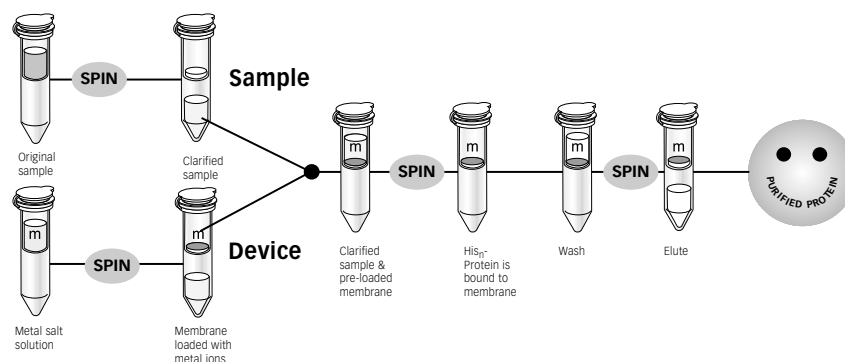

Protocol for Vivapure Metal Chelate Mini spin columns

Additional equipment required:

Hardware: Any micro-centrifuge that will accommodate 2 ml centrifuge tubes and can spin samples at speeds up to 2000 x g.

Buffers and aqueous metal salt solutions: Please refer to the section, "Recommended buffers" and "Recommended aqueous metal salt solutions".

Optional devices for highly diluted samples: Vivaspin 2 or Vivaspin 4

If your original sample is highly diluted, you can reduce the sample volume preceding the sample clarification step described below. We recommend Vivaspin 2, 10 kDa MWCO (Vivascience catalog No. VS0201 or VS0202) for sample volumes up to 2 ml or Vivaspin 4 (Vivascience catalog No. VS0403 or VS0404) for volumes up to 4 ml.

Sample preparation

Prepare the cell lysates according to your standard protocol (sodium phosphate is recommended as buffer system for cell lysis) and subsequently continue with the step "Sample clarification" described below.

For more detailed information on the preparation of cell lysates, please refer to general information sources like "Current Protocols in Molecular Biology" by Frederick M. Ausubel, Roger Brent, Robert E. Kingston, David D. Moore, J. G. Seidman, Kevin Struhl.

Sample clarification

To avoid clogging of the Vivapure Metal Chelate Mini spin column, the original sample should be pre-filtered before it is loaded onto the Vivapure Mini spin column. Pre-filtration is performed using the Clarification Mini spin column.

1. Pipette up to 400 µl of the sample onto the Clarification Mini spin column. Spin for 5 min at 2000 x g. The flow-through represents the clarified sample.

(For sample volumes higher than 400 µl, the Clarification Mini spin column can be re-loaded until the whole sample is clarified.)

Store the clarified sample on ice or under appropriate conditions and pre-load the membrane of the Vivapure Metal Chelate Mini spin column with metal ions (next step).

PLEASE NOTE THAT PRE-LOADING OF THE MEMBRANE WITH METAL IONS SHOULD TAKE PLACE IMMEDIATELY BEFORE SAMPLE PURIFICATION!

Membrane pre-loading with metal ions:

As described above, various metal ions can be bound to the chelate membrane. We recommend using nickel (Ni⁺⁺), cobalt (Co⁺⁺), copper (Cu⁺⁺) or zinc (Zn⁺⁺) ions for purification. Nevertheless, depending on the particular application, even better results may be achieved with other metal ions. See also section "Recommended aqueous metal salt solutions".

1. Prepare the 0.5 M salt solution(s) of your choice as described above.
2. Pre-wet the Vivapure Metal Chelate Mini spin column with 400 µl distilled water. Spin for 1 min at 1500 x g and discard the flow-through.
3. Load 400 µl of a 0.5 M aqueous metal salt solution. Spin for 1 min at 1500 x g and discard the flow-through. Repeat this step.
4. Fill in 400 µl distilled water and spin for 1 min at 1500 x g to remove unbound metal ions. Repeat this step.

Now the Vivapure Metal Chelate Mini spin column is ready for sample loading.

Sample loading and purification

1. Equilibrate the membrane with 400 µl equilibration buffer. Spin for 1 min at 1500 x g and discard the flow-through. Repeat this step.
2. Load up to 400 µl sample solution onto the membrane. Centrifuge for 3 min at 1500 x g. For sample volumes higher than 400 µl, the Vivapure Metal Chelate Mini spin column can be re-loaded to bind your complete sample as long as the membrane capacity is considered.
3. Wash the membrane with 400 µl washing buffer. Spin for 3 min at 1500 x g and discard the flow-through. Repeat this step.
Note: An optional third washing step might be included to increase purity.
4. Pipette 200 µl elution buffer onto the membrane to elute the protein. Spin for 3 min at 1500 x g. The flow-through contains the purified protein.
5. A second and third elution step with 400 µl elution buffer may be necessary to elute all of the desired protein.

Optional concentration or buffer exchange after elution:

For subsequent applications, is often useful to further concentrate the eluate or to exchange the buffer in the eluate. Both applications can be easily and conveniently performed using Vivaspin 500, 10 kDa MWCO (Vivascience catalog No. VS0101 or VS0102), if the total elution volume does not exceed 500 µl. For larger total elution volumes we recommend Vivaspin 2, 10 kDa MWCO (Vivascience catalog No. VS0201 or VS0202) or Vivaspin 4, 10 kDa MWCO (Vivascience catalog No. VS0403 or VS0404).

Recommended aqueous metal salt solutions:

Pre-loading with metal ions, choice of optimal metal ion for your purification.

→ See Table 1 below

Vivapure Metal Chelate Mini spin columns were specifically designed to allow you choose the metal ions to be immobilized on the membrane. If there is little prior knowledge about the purification of your poly-histidine tagged target protein, we recommend to start with nickel (Ni^{++}), cobalt (Co^{++}), copper (Cu^{++}) or zinc (Zn^{++}) ions.

For the initial run, you can either use one of the metal ion solutions described in Table 1, or screen all four metal ion solutions in parallel to find the best performing for your application. In this case, please use one Vivapure Metal Chelate Mini spin column for each aqueous metal ion solution.

For certain proteins or applications, the use of different metal ions apart from nickel (Ni^{++}), cobalt (Co^{++}), copper (Cu^{++}) or zinc (Zn^{++}) may increase the degree of purity. If further optimization is desired, different metal ions like ferrous (Fe^{++}) or cadmium (Cd^{++}) can also be tested.

Table 1: Recommended aqueous solutions of Ni^{++} , Co^{++} , Cu^{++} or Zn^{++} ions for the step "Membrane pre-loading with metal ions"

Ni^{++}	0.5 M Nickel sulphate (e.g. $\text{NiSO}_4 \cdot 6\text{H}_2\text{O}$) in deionized water
Co^{++}	0.5 M Cobalt chloride (e.g. $\text{CoCl}_2 \cdot 6\text{H}_2\text{O}$) in deionized water
Cu^{++}	0.5 M Copper sulphate (e.g. CuSO_4 or $\text{CuSO}_4 \cdot 5\text{H}_2\text{O}$) in deionized water
Zn^{++}	0.5 M Zinc chloride (e.g. ZnCl_2) in deionized water

Recommended buffers for equilibration, washing and elution:

→ See Table 2 below

As mentioned above, expression systems for proteins with poly-histidine tags are highly diverse. Therefore, the described purification buffers should be considered only as guidelines. For the best performance and recovery, we recommend optimization of conditions for the individual target protein.

Contaminating proteins in the eluate can be reduced by varying the imidazole concentration in the washing buffer. If the poly-histidine tagged protein cannot be detected after elution with 250 mM imidazole, the imidazole concentration of the elution buffer should be increased. Depending on the elution conditions, leaching of the metal ions from the membrane may occur.

We recommend the following buffers for purifying the protein of interest under native conditions - see Table 2.

Table 2: Buffer recommendations for purification under native conditions*

Equilibration buffer:

50 mM NaH₂PO₄, 300 mM NaCl, 10 mM imidazole, pH 8.0*

Washing buffer:

50 mM NaH₂PO₄, 300 mM NaCl, 20 mM imidazole, pH 8.0*

Elution buffer:

50 mM NaH₂PO₄, 300 mM NaCl, 250 mM imidazole, pH 8.0*

* Under denaturing conditions 8 M urea may be added.

Ordering Information

Cat Number	Vivapure Spin Columns	Spin Columns	Cat Number	Vivapure Ion Exchange Maxi Spin Columns	Spin Columns	Centrifuge Tubes	
VS-PA01PA24	Protein A Mini	24	VS-IX20CM08	Vivapure C Maxi M	8	16	
VS-MC01MC12	Metal Chelate Mini	12	VS-IX20CH08	Vivapure C Maxi H	8	16	
Cat Number	Vivapure Kits	Spin Columns	VS-IX20DM08	Vivapure D Maxi M	8	16	
VS-PC01EPPC	Epoxy Protein Coupling Kit	12	VS-IX20DH08	Vivapure D Maxi H	8	16	
VS-IX01QHGP	Acidic Protein Purification Kit Q Mini H	8	VS-IX20QM08	Vivapure Q Maxi M	8	16	
VS-IX20QHGP	Acidic Protein Purification Kit Q Maxi H	4	VS-IX20QH08	Vivapure Q Maxi H	8	16	
VS-IX01SHGP	Basic Protein Purification Kit S Mini H	8	VS-IX20SM08	Vivapure S Maxi M	8	16	
VS-IX20SHGP	Basic Protein Purification Kit S Maxi H	4	VS-IX20SH08	Vivapure S Maxi H	8	16	
VS-IX01QHAR	Albumin Removal Kit Q Mini H	12	Cat Number	Vivapure Ion Exchange Mega Spin Columns	Spin Columns	Centrifuge Tubes	
VS-IX20QHAR	Albumin Removal Kit Q Maxi H	4	VS-IX75QH02	Vivapure Q Mega H	2	2	
VS-IX01DMDR	DNA Removal Kit D Mini M	12	VS-IX75DH02	Vivapure D Mega H	2	2	
VS-IX20DMDR	DNA Removal Kit D Maxi M	6	VS-IX75SH02	Vivapure S Mega H	2	2	
Cat Number	Vivapure Ion Exchange Mini Spin Columns	Spin Columns	Centrifuge Tubes	VS-IX75CH02	Vivapure C Mega H	2	2
VS-IX01ST16	Vivapure Mini H Starter Kit (4 of each ion exchange class)	16	32				
VS-IX01CL24	Vivapure C Mini L	24	48				
VS-IX01CM24	Vivapure C Mini M	24	48				
VS-IX01CH24	Vivapure C Mini H	24	48				
VS-IX01DL24	Vivapure D Mini L	24	48				
VS-IX01DM24	Vivapure D Mini M	24	48				
VS-IX01DH24	Vivapure D Mini H	24	48				
VS-IX01QL24	Vivapure Q Mini L	24	48				
VS-IX01QM24	Vivapure Q Mini M	24	48				
VS-IX01QH24	Vivapure Q Mini H	24	48				
VS-IX01SL24	Vivapure S Mini L	24	48				
VS-IX01SM24	Vivapure S Mini M	24	48				
VS-IX01SH24	Vivapure S Mini H	24	48				

For more information on related products, please refer to the:

- Vivascience Ultrafiltration Catalog - Vivaspin
- Vivapure® Catalog for kits and devices for protein purification
- Vivapure® Protein A Mini spin column brochure
- Vivapure® Epoxy Protein Coupling kit brochure
- Vivascience Cell Culture Catalog

For current information and application notes, please visit us at www.vivascience.com

Vivascience Technical Support		Phone	Fax	E-mail
USA	Vivascience Service & Technical Support	+1 877 452 2345 (toll free)	+1 760 918 8281	info.usa@vivascience.com
Europe	Vivascience Support Center	+49 1 802 000 581 (toll free)	+49 1 802 000 583	info@sc.vivascience.de
International	Vivascience Support Center	+49 551 38906 0	+49 551 38906 11	info@sc.vivascience.de
Vivascience Customer Sales				
France	Vivascience S.A.R.L.	+33 169 19 93 23	+33 160 13 95 05	info.france@vivascience.com
Germany	Vivascience AG	+49 551 308 4023	+49 551 308 3289	info.germany@vivascience.com
UK	Vivascience Ltd.	+44 1372 737 159	+44 1372 726 171	info.uk@vivascience.com
USA	Vivascience Inc.	+1 877 452 2345	+1 760 918 8281	info.usa@vivascience.com

Vivascience AG

Feodor-Lynen-Strasse 21 Phone: +49 511 524875-0 E-mail: info@vivascience.com
 30625 Hannover, Germany Fax: +49 511 524875-19 Web: www.vivascience.com

The information in this publication is believed to be accurate, and is offered in good faith for the benefit of the user. As we cannot anticipate or control conditions of product application, we do not warrant suitability or favourable results, nor that use will not infringe on any patents. Products are furnished upon the condition that the user assumes all risks and liabilities and that neither seller or manufacturer shall be liable for any loss or damage, direct or sequential arising from the use or inability to use the product. Specifications subject to change without notice. © 2002 Vivascience Ltd. Publication No. SL-2016-e03011. Order No. 85030-516-98.